Towards Assurance of a Patient-Specific Network of Medical Devices.

SCC 2015, Rockville Maryland

Sam Procter, John Hatcliff, and Robby
SAnToS Lab
Kansas State University

Support:

This work is supported in part by the US National Science Foundation (NSF) (#1239543), the NSF US Food and Drug Administration Scholar-in-Residence Program (#1355778) and the National Institutes of Health / NIBIB Quantum Program.

Health Care Involves A Variety of System Components

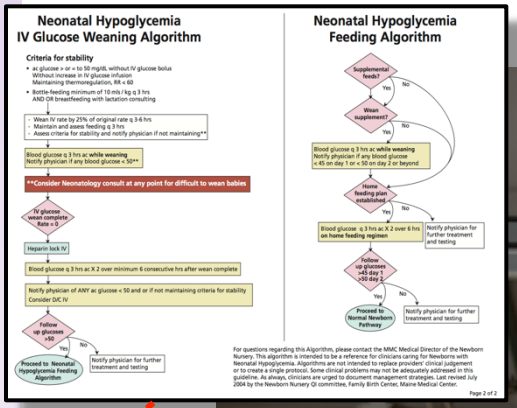

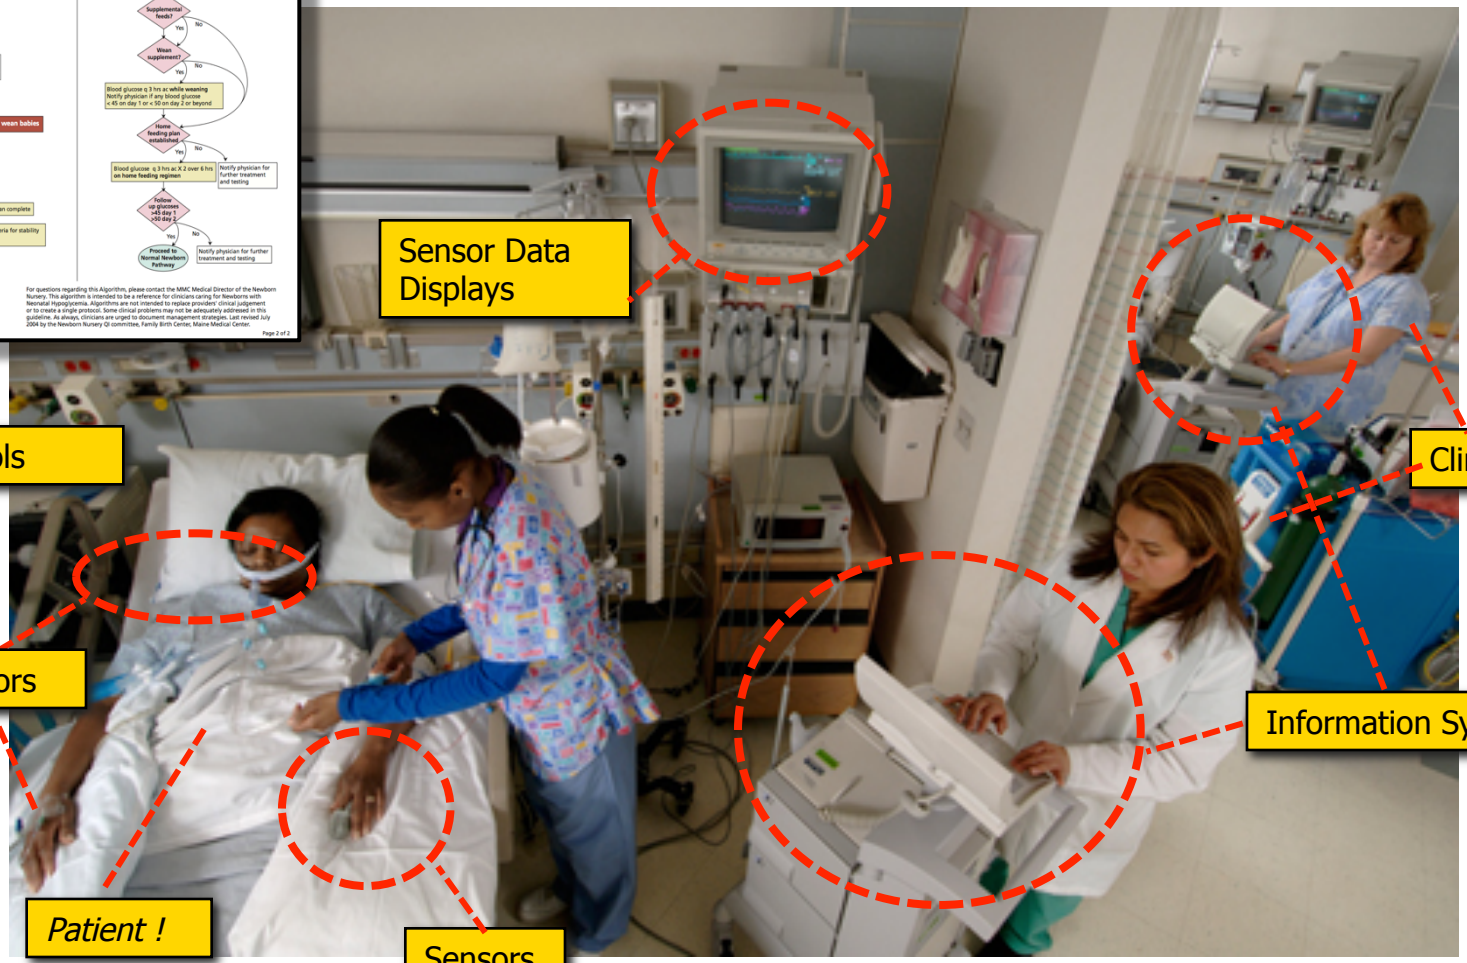

Clinical Protocols

Sensor Data Displays

Clinicians

Actuators

Information Systems

Patient !

Sensors

Motivation

- What are the types of things we could do with device integration?
  - Information forwarding
  - Automation of clinical workflows
  - Closed loop control between devices
- Unlike personal computing, medical devices are not designed to work together
- Integrating medical devices would bring myriad benefits

- … how can we do so safely?

Outline

- Background
  - PCA Interlock Scenario
  - Medical Application Platforms
  - Tooling
- Status Quo
- STPA + AADL
- Impacts / Future

PCA Interlock Scenario

- Patients are commonly given patient-controlled analgesics after surgery
- Crucial to care, but numerous issues related to safety
- Data for disabling the pump exists now (just a system invariant) -- we just need to integrate it

PCA Pump Safety Interlock

Fully leverage device data streams and the ability to *control* devices

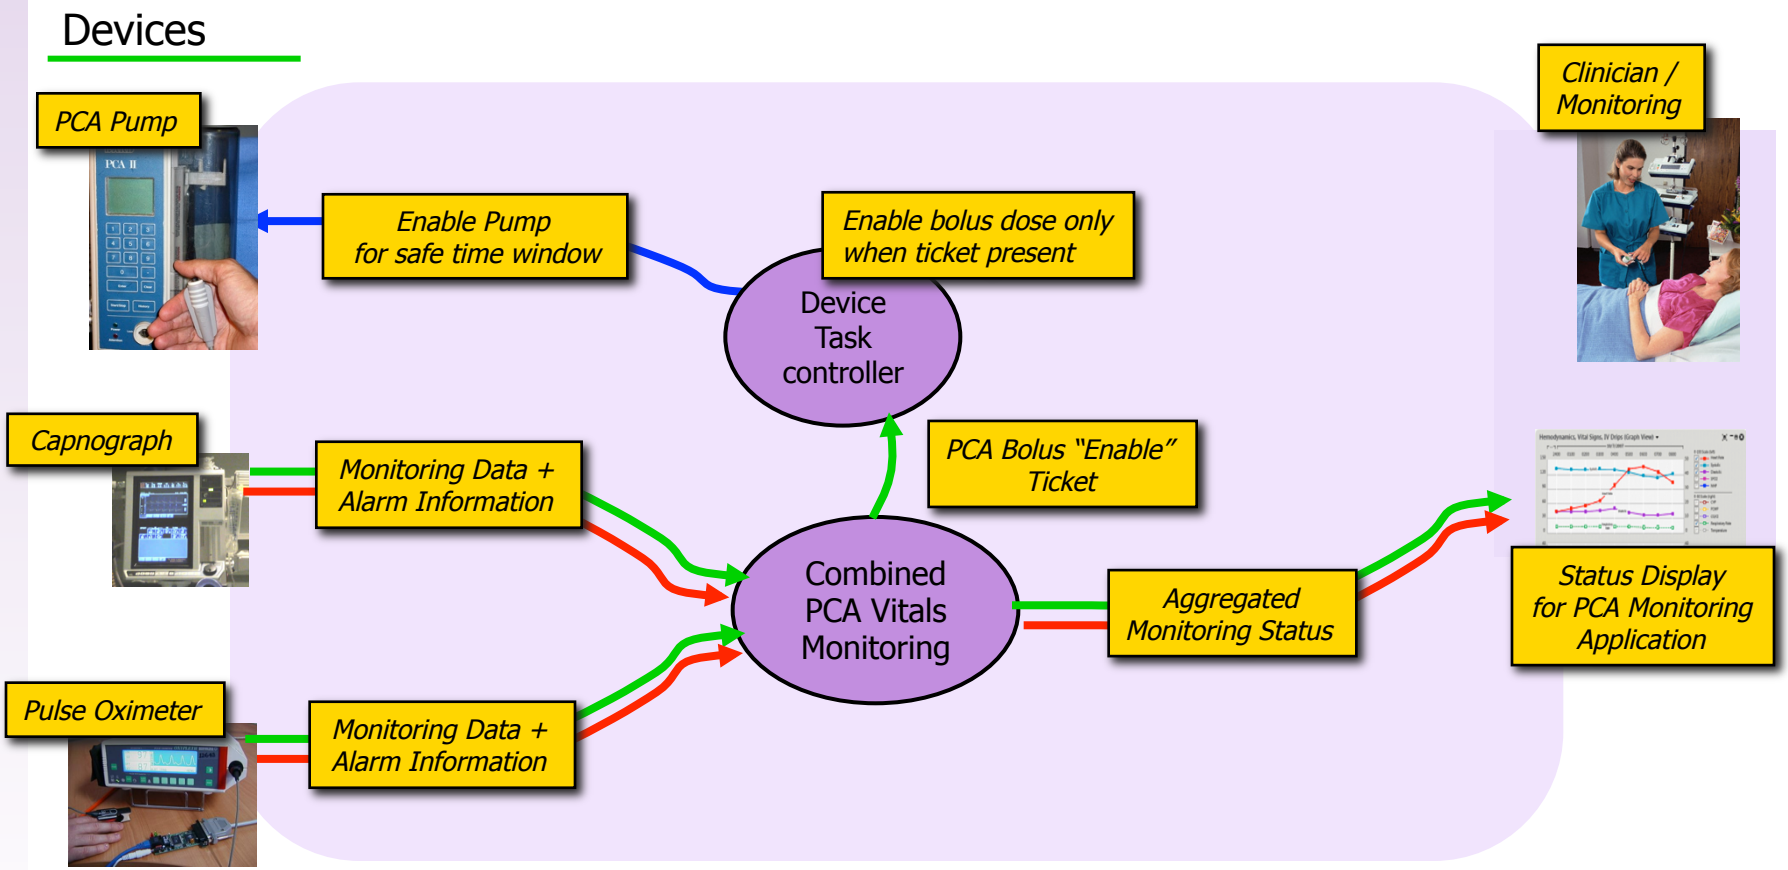

Medical Application Platforms

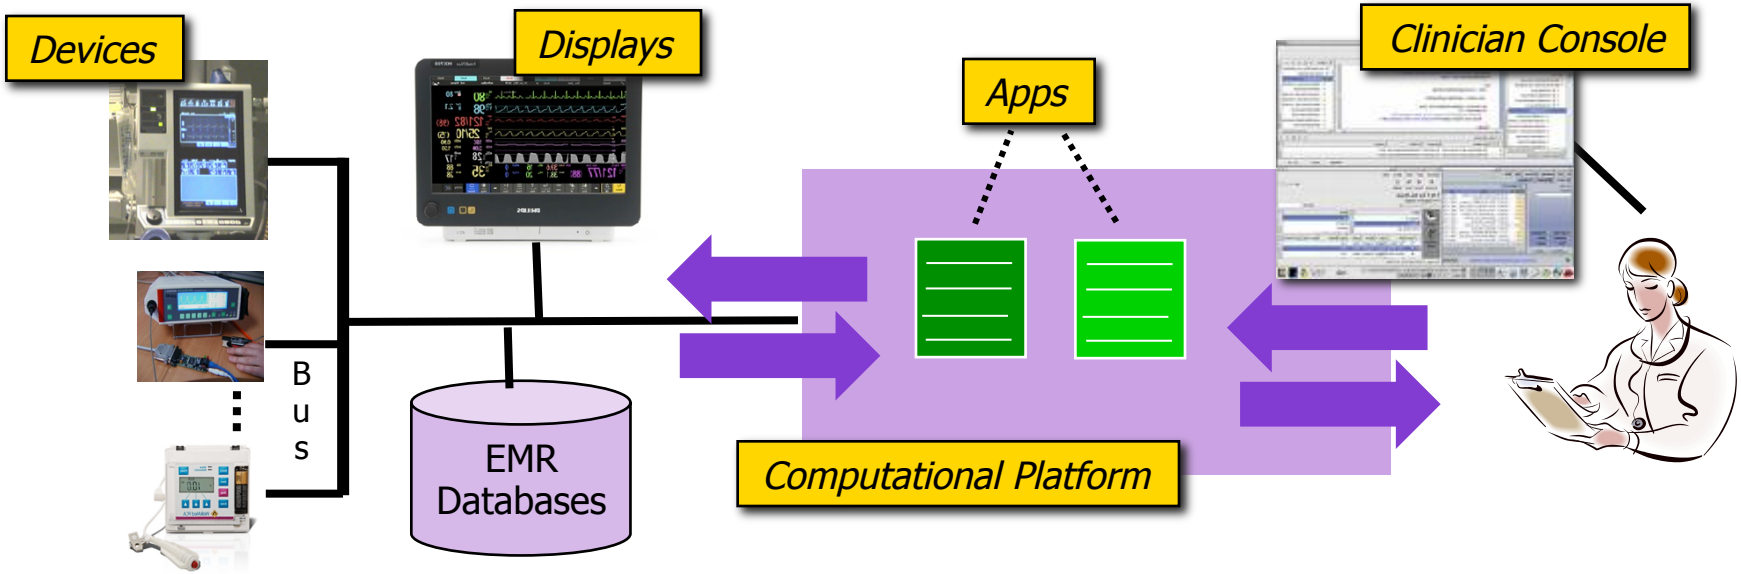

- A *Medical Application Platform* is a safety- and security-critical real-time computing platform for…
  - Integrating heterogeneous devices, medical IT systems, and information displays via communications infrastructure, and
  - Hosting applications (“apps”) that provide medical utility via the ability to acquire information from and update/control integrated devices, IT systems, and displays

Extension beyond medicine

- We use medicine in our examples
  - … but this can extend to other compositional systems
- Core idea:
  - Integration of heterogeneous
    - Sensors,
    - Actuators, and
    - Complete systems,
  - by small chunks of software,
  - in a verifiable manner

Background

PCA Pump Interlock Architecture

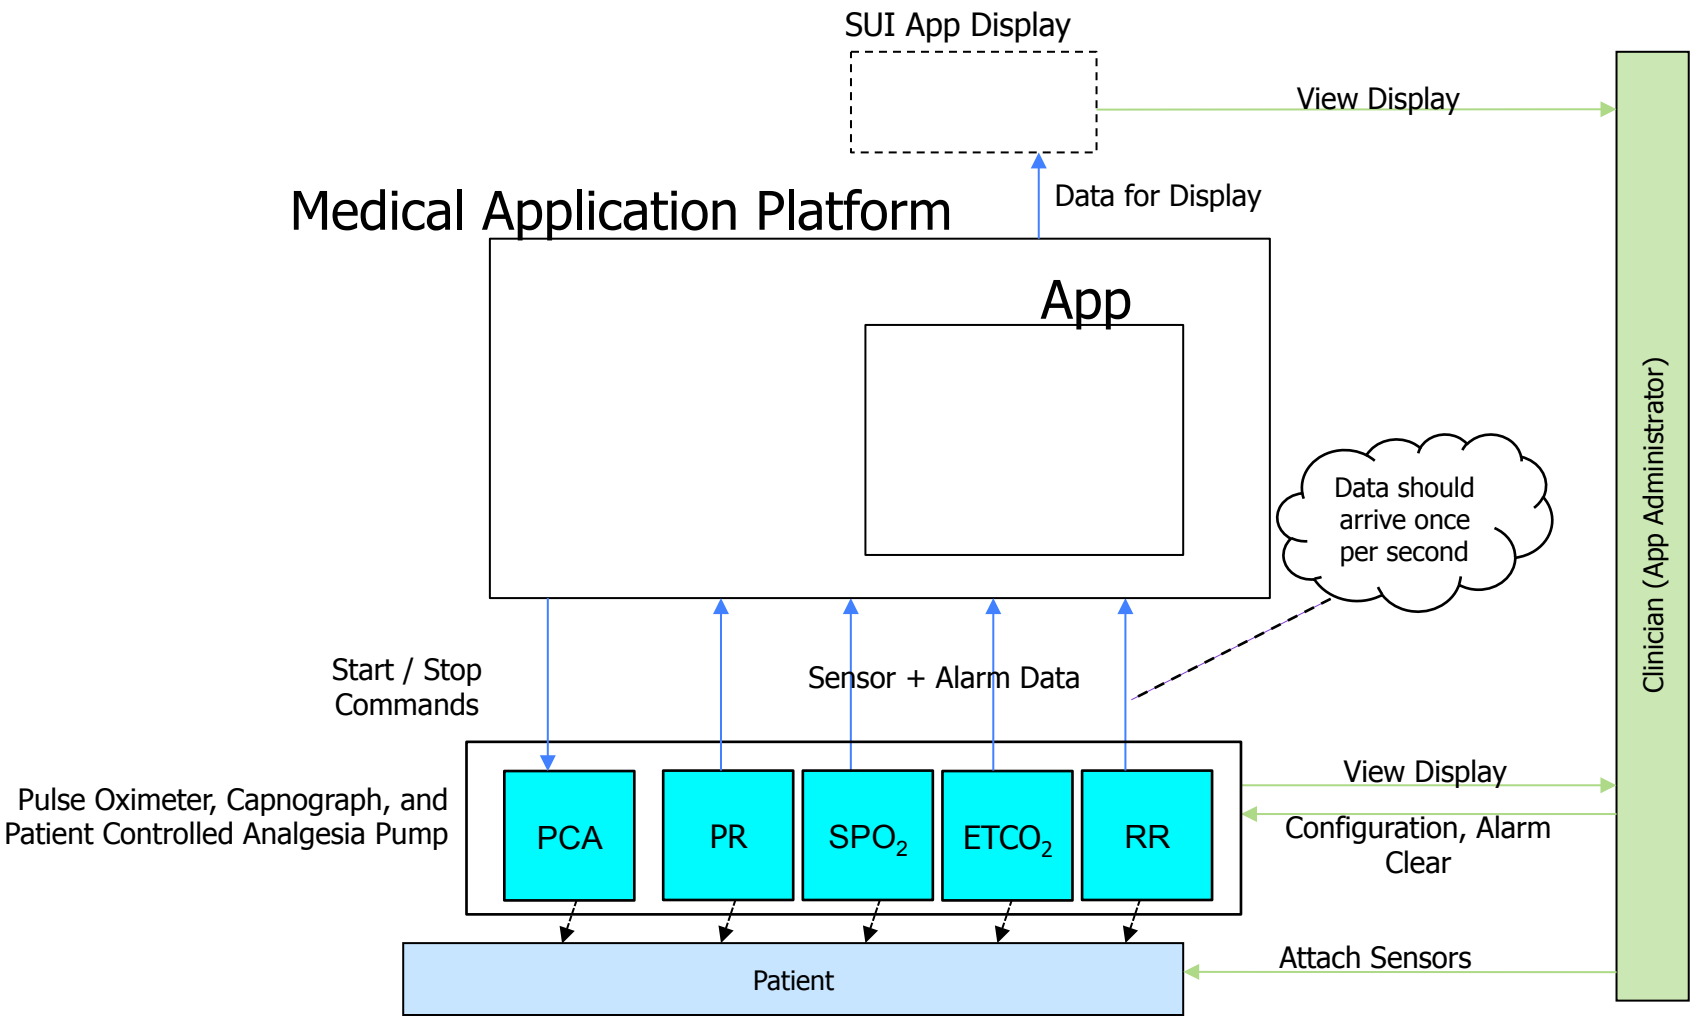

Tooling Vision

Analyses and Regulatory Artifacts

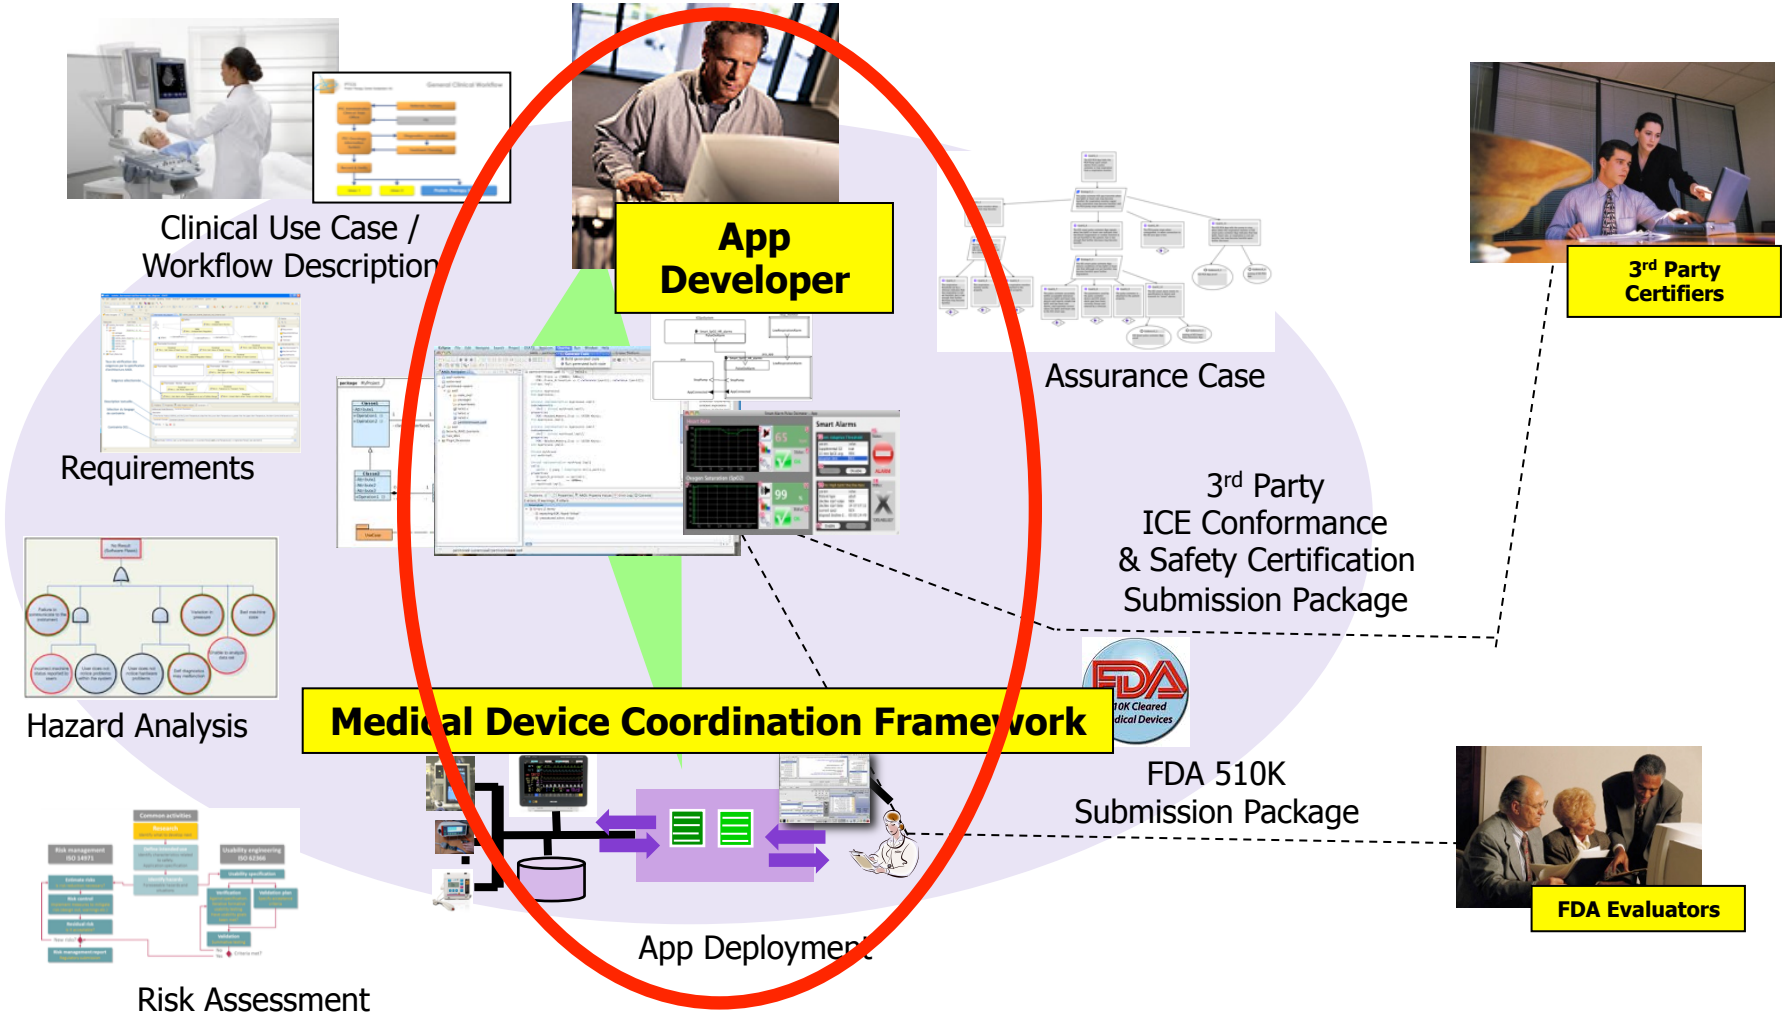

Tooling Vision

Code Generation

A. The app's architecture is specified in a suitable formalism
   1. Components as AADL Devices / Processes
   2. Connections are specified
   3. RT/QoS Parameters are via AADL's property-specification mechanism

B. The app is programmatically translated to Java and XML
   1. Only "Business Logic" is written by the developer

C. The app is launched on a compatible MAP

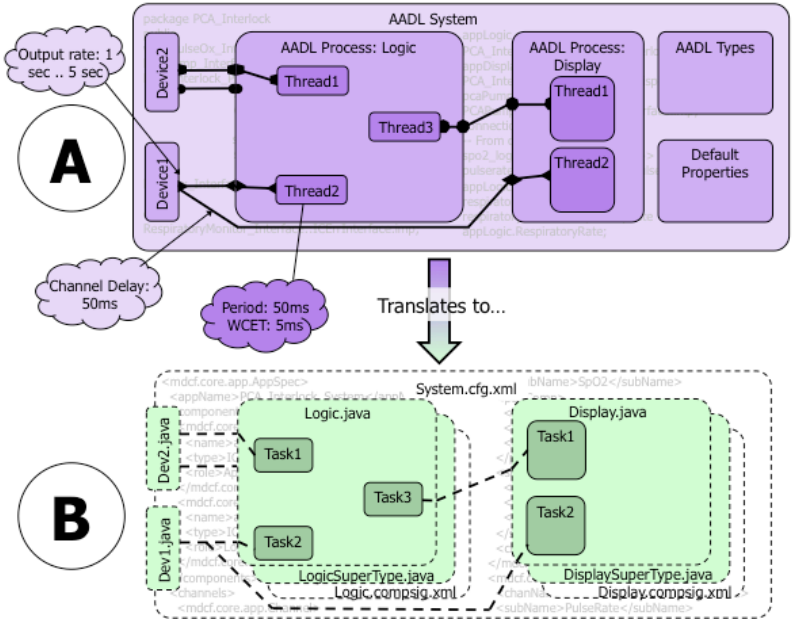

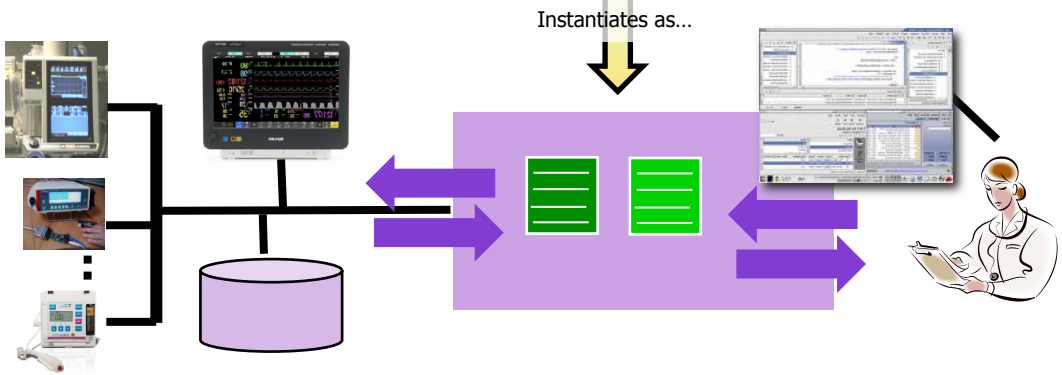

Component Development

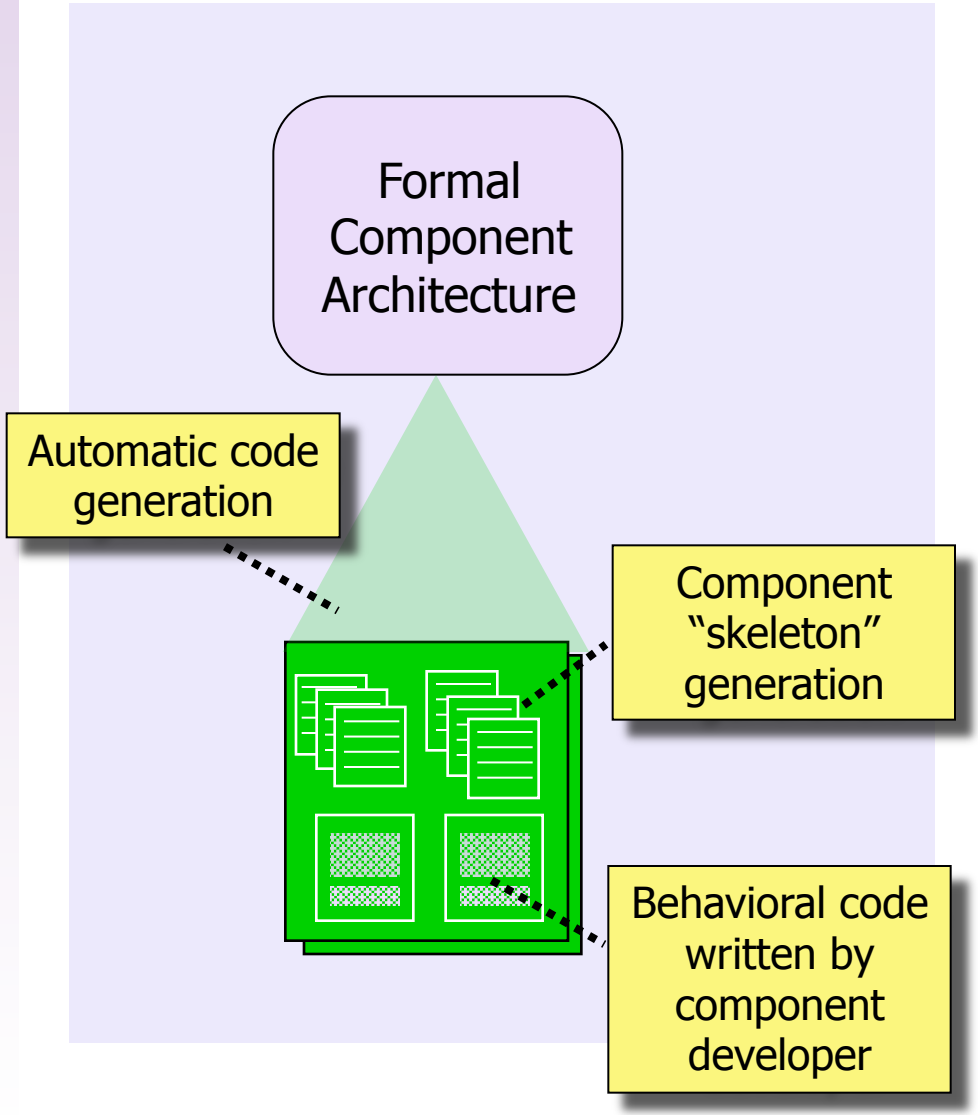

- Development of component architecture using architecture formalism
- Automatic generation of component architecture (skeletons)
- Automatic generation of component layout and app topology (configuration)
- Development of core behavioral code (business logic) using IDE of choice
- Translator can be retargeted to other languages as desired

Outline

- Background
- Status Quo
  - Existing Hazard Analyses
  - Application to MAP domain
- STPA + AADL
- Impacts / Future

Hazard Analysis

History: FTA

- FTA: Bell Labs, 1962
  - Looks for contributory causes to undesired events

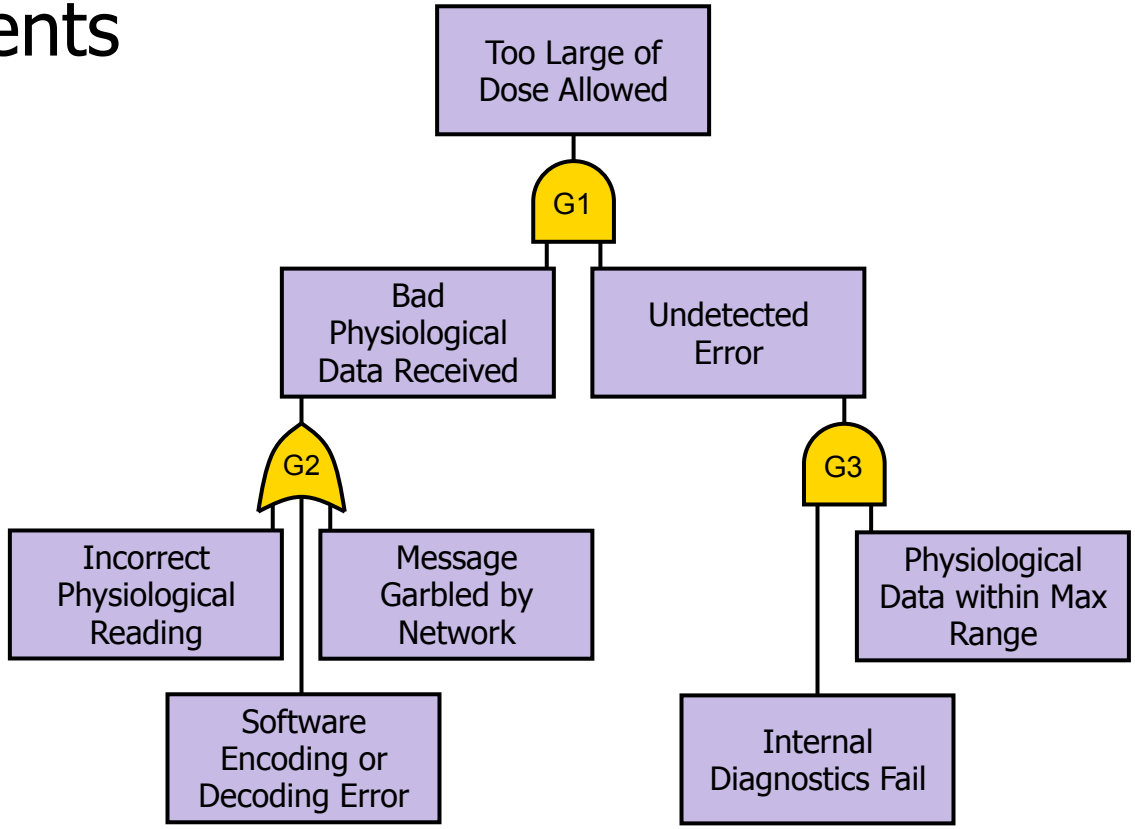

Hazard Analysis

History: FMEA

- FMEA: US Military, 1949
  - Analyses impacts of individual components

System: PCA Interlock Scenario			Subsystem: Pulse Oximeter Device				Mode/Phase: Execution			
Function	**Failure Mode**	**Fail Rate**	**Causal Factors**	**Effect**	**System Effect**	**Detected by**	**Current Control**	**Hazard**	**Risk**	**Rec. Action**
Provide SpO_2	Fails to Provide	N/A	Network or dev. Failure	No SpO_2 data	Unknown patient state	App		Potential OD	3D	Default to KVO
	Provides late	N/A	Network slowness	No SpO_2 data	Unknown patient state	App		Potential OD	3C	Default to KVO
	Provides wrong	N/A	Device error	SpO_2 wrong	Wrong patient state	None		Potential OD	1E	Dev. should report data quality
Analyst: Sam Procter			Date: September 26, 2014				Page 3/14			

Unique aspects of MAP domain

- Software based
  - Hardware is interchangeable
- Component oriented
  - Compositional system needs compositional safety
- Unclear how FTA / FMEA might apply
- Early, firm notion of system architecture

Formalized Notion of Architecture

- Formal architecture descriptions become the scaffolding on which:
  - Requirements,
  - Development,
  - Risk management,
  - Deployment, and
  - Ecosphere coordination is organized.

Outline

- Background
- Status Quo
- STPA + AADL
  - STPA
  - AADL
  - Tool-based Integration: MDCF Architect
- Impacts / Future

Hazard Analysis

Leveraging Semiformal Architectural Descriptions

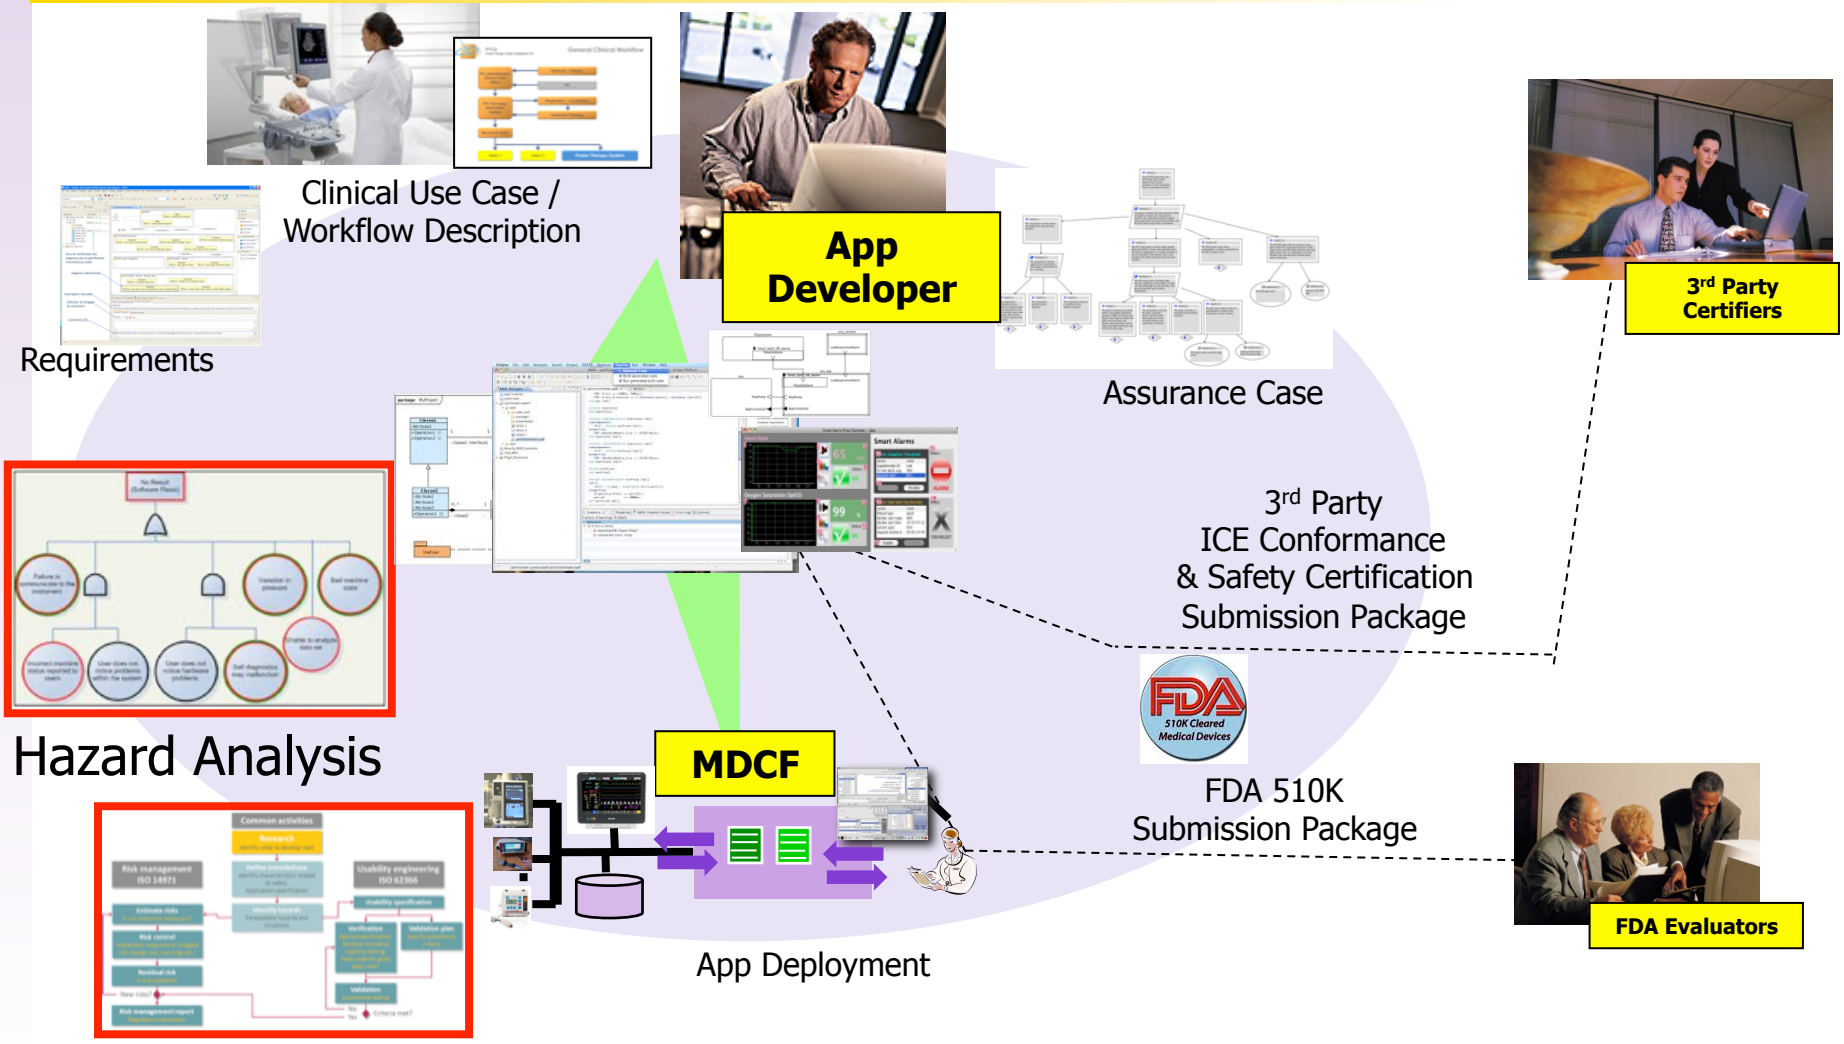

Hazard Analysis

History: STPA

- STPA: Nancy Leveson / MIT, 2005(ish)
- Applies systems theory, focuses on control…
  - Loops
  - Actions

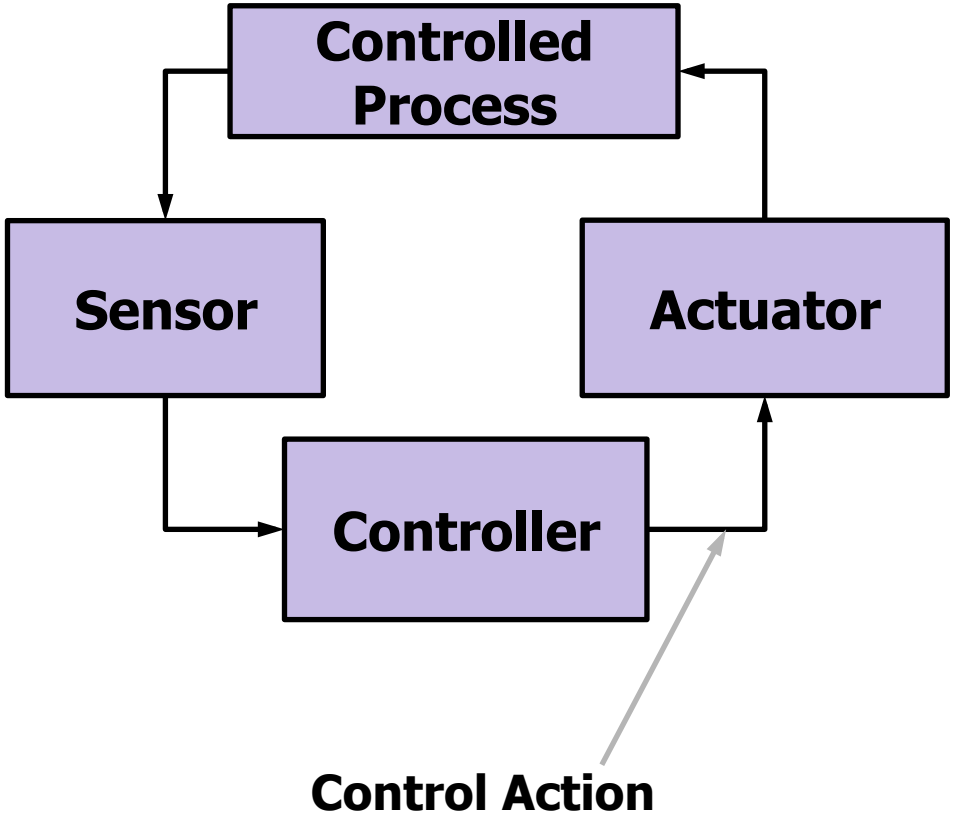

Hazard Analysis

History: STPA

- STPA: Nancy Leveson / MIT, 2005(ish)
- Applies "Systems" theory, focuses on control…
  - Loops
  - Actions

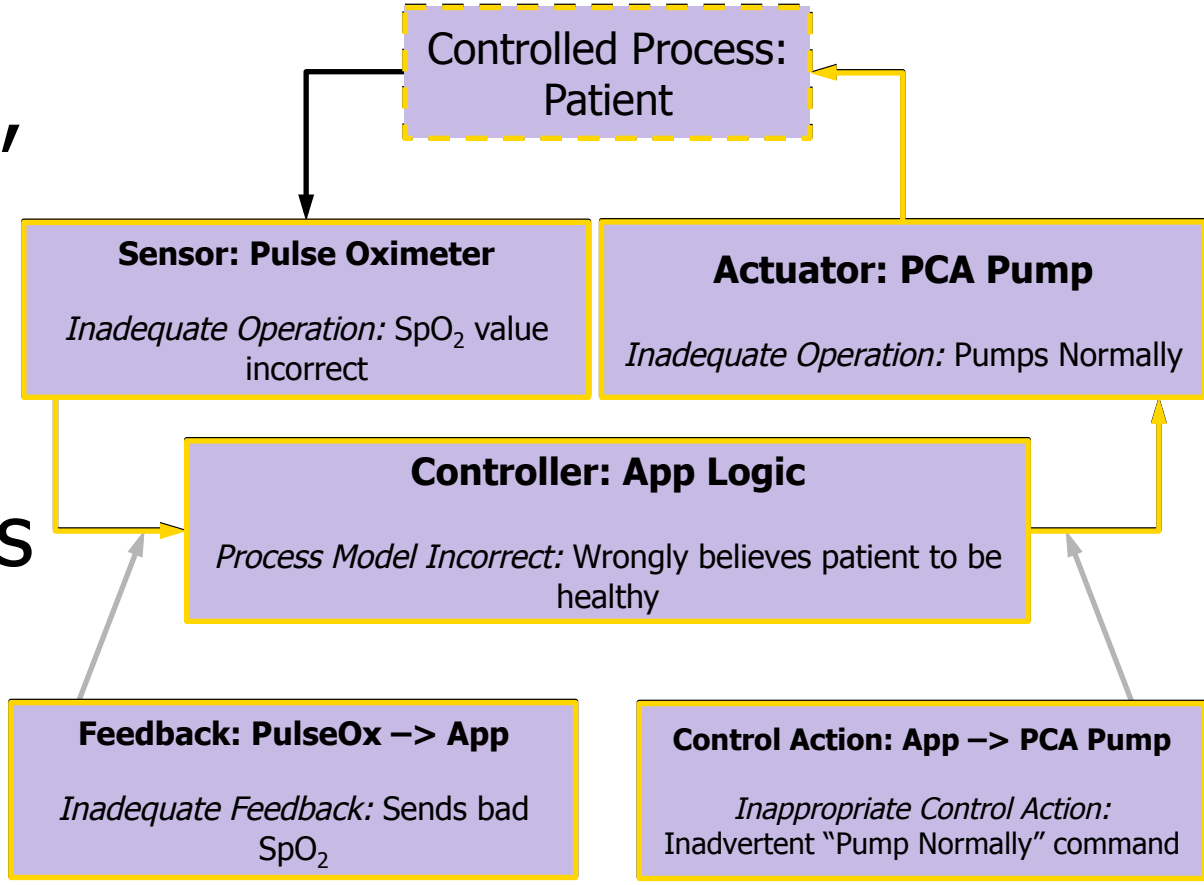

Hazard Analysis

Can STPA be improved?

- STPA enables reasoning about
  - Hardware,
  - Software, and
  - Socio-technical elements
- And is driven by architecture ("Boundary Crossing")
- No open tooling
  - Tooling isn't bound to architecture
- Existing work is largely manual

Language

Why use AADL?

- *Architecture* Analysis and Design Language
- History of successful safety-critical projects
  - Avionics / Boeing (SAVI): “integrate-then-build” approach
- Annexes support a number of regulatory and verification artifacts
  - Hazard Analysis (EM) extends notion of interface to include faults

Language

Model

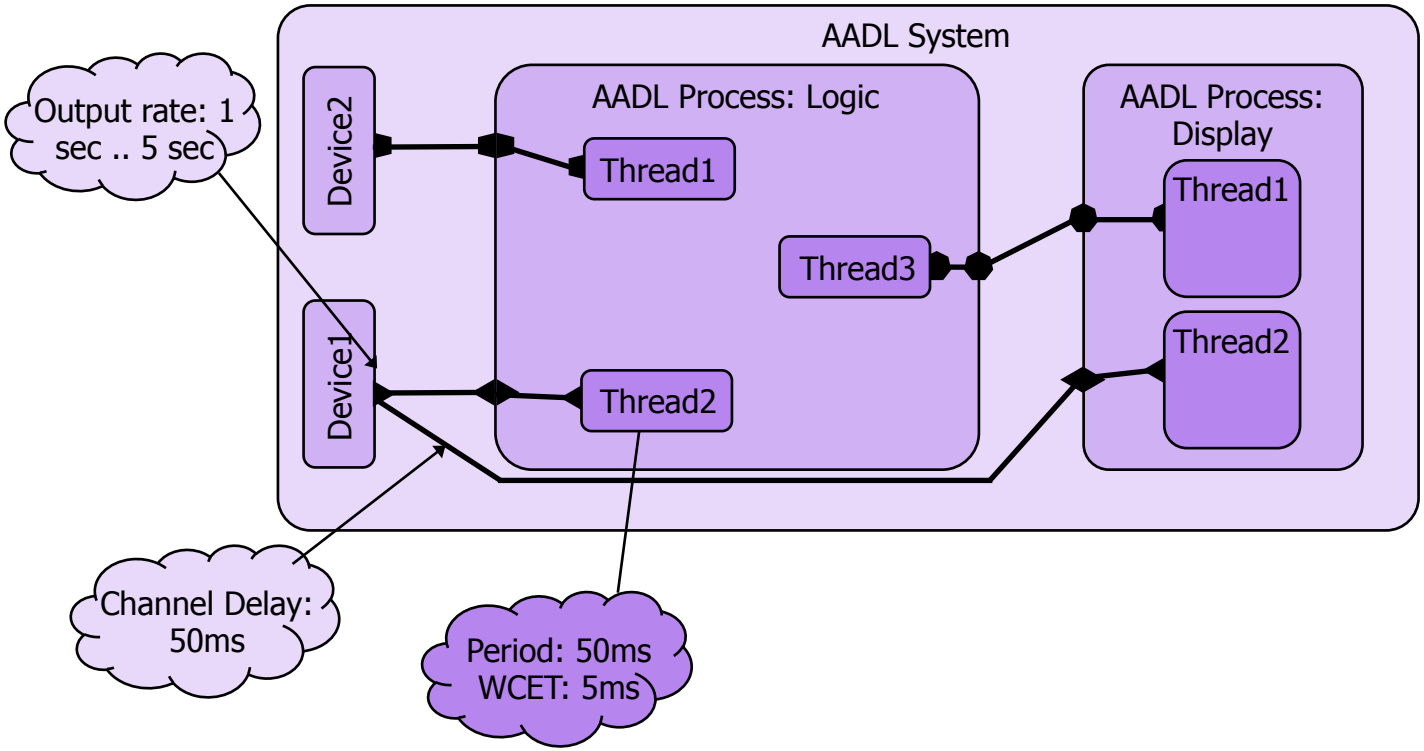

Language

System

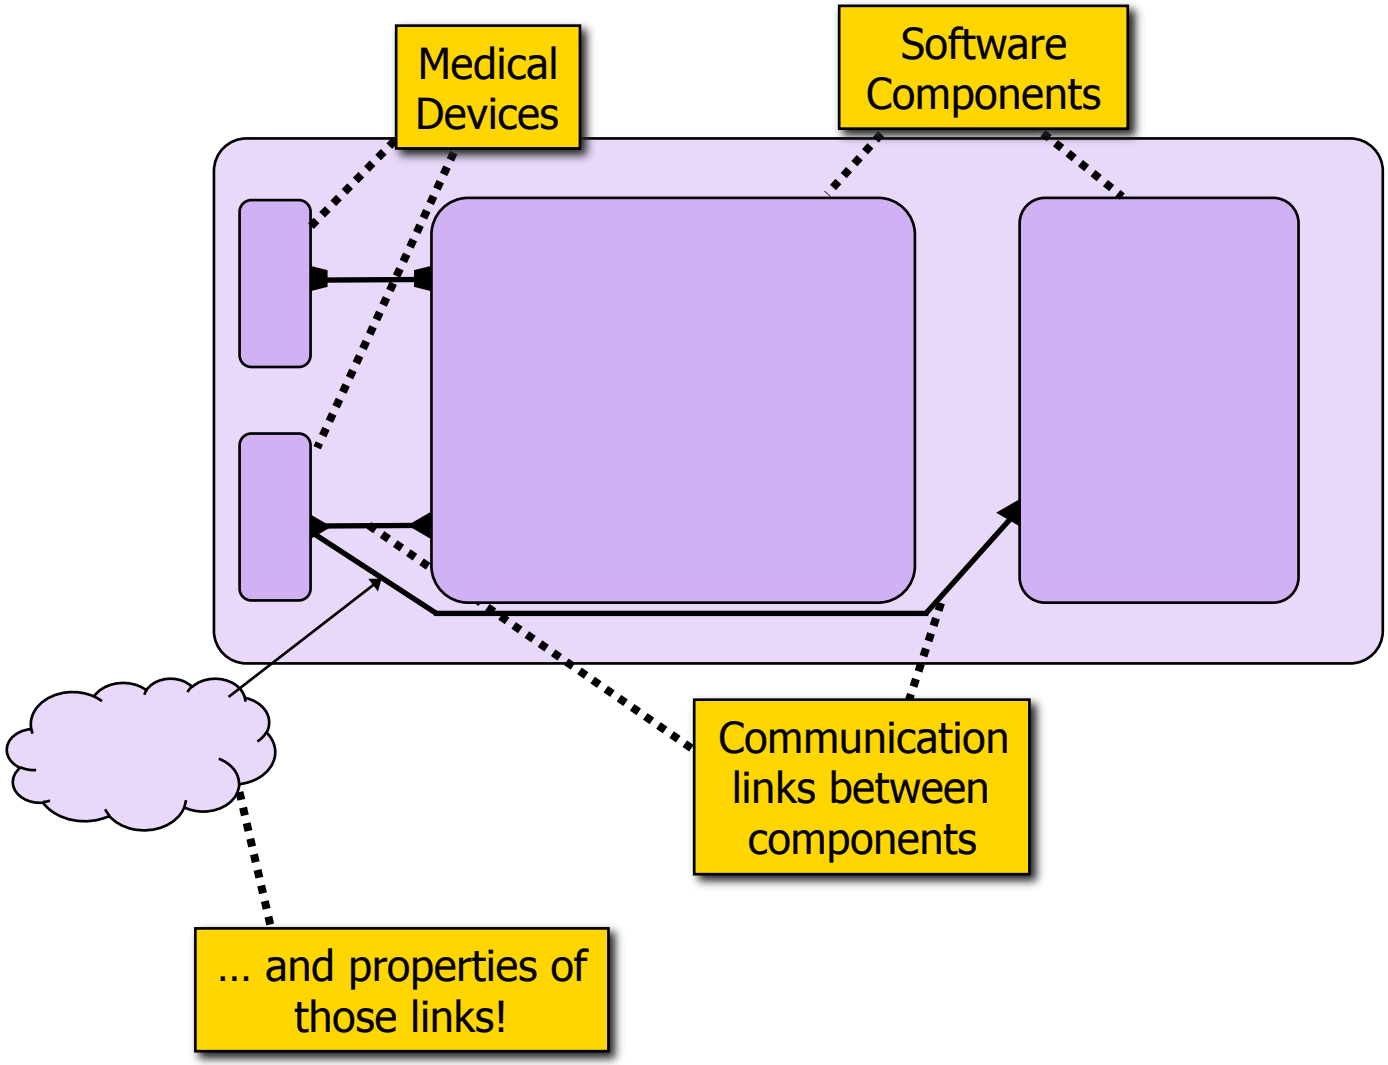

Language

System

```
package PCA_Shutoff
public
with PulseOx_Interface, PCAPump_Interface, PCA_Shutoff_Logic,
        PCA_Shutoff_Properties, MAP_Error_Properties, PCA_Shutoff_Display,
        PCA_Shutoff_Errors, Capnograph_Interface, MAP_Errors,
        PCA_Shutoff_Error_Properties;

        system PCA_Shutoff_System
        end PCA_Shutoff_System;

        system implementation PCA_Shutoff_System.imp
        subcomponents
                -- Physiological inputs
                capnograph : device Capnograph_Interface::ICEcapnographInterface.imp;

                -- App logic
                appLogic : process PCA_Shutoff_Logic::ICEpcaShutoffProcess.imp;
                appDisplay : process PCA_Shutoff_Display::ICEpcaDisplayProcess.imp;

                -- Controlled device
                pcaPump : device PCAPump_Interface::ICEpcaInterface.imp;
        connections
                -- From components to logic
                respiratoryrate_logic : port capnograph.RespiratoryRate -> appLogic.RespiratoryRate;
                pumpcommand_logic : port appLogic.CommandPumpNormal -> pcaPump.PumpNormally;
                etco2_logic : port capnograph.ETCO2 -> appLogic.ETCO2
                {MAP_Properties::Channel_Delay => 50 ms;};

                -- From components to display
                pumpcommand_disp : port appLogic.CommandPumpNormal -> appDis
        end PCA_Shutoff_System.imp;

end PCA_Shutoff;
```

Medical Devices

Software Components

Communication links between Components

… and properties of those links!

STPA: Fundamentals

- Fundamentals
  - Accident Levels
  - Accidents
  - System Boundaries
  - Hazards
  - Safety Constraints
  - Control Actions
  - Control Structure

Hazard Analysis

STPA: Fundamentals

- Fundamentals
  - Accident Levels
  - Accidents
  - System Boundaries
  - Hazards
  - Safety Constraints
  - Control Actions
  - Control Structure

Example

1. A human is killed or seriously injured.
2. A medical device's services are unavailable

```
DeathOrInjury : constant MAP_Error_Properties::Accident_Level => [
        Level => 1;
        Description => "A human is killed or seriously injured.";
];
```

Tie into ISO 14971's notions of criticality?

Hazard Analysis

STPA: Fundamentals

- Fundamentals
  - Accident Levels
  - Accidents
  - System Boundaries
  - Hazards
  - Safety Constraints
  - Control Actions
  - Control Structure

Example

1. The patient is killed or seriously injured [DeathOrInjury]

2. The PCA pump stops responding to commands [DenialOfService]

```
PatientHarmed : constant MAP_Error_Properties::Accident => [
        Number => 1;
        Description => "Patient is killed or seriously injured.";
        Level => PulseOx_Forwarding_Error_Properties::DeathOrInjury;
];
```

Hazard Analysis

STPA: Fundamentals

- Fundamentals
  - Accident Levels
  - Accidents
  - System Boundaries
  - Hazards
  - Safety Constraints
  - Control Actions
  - Control Structure

Example

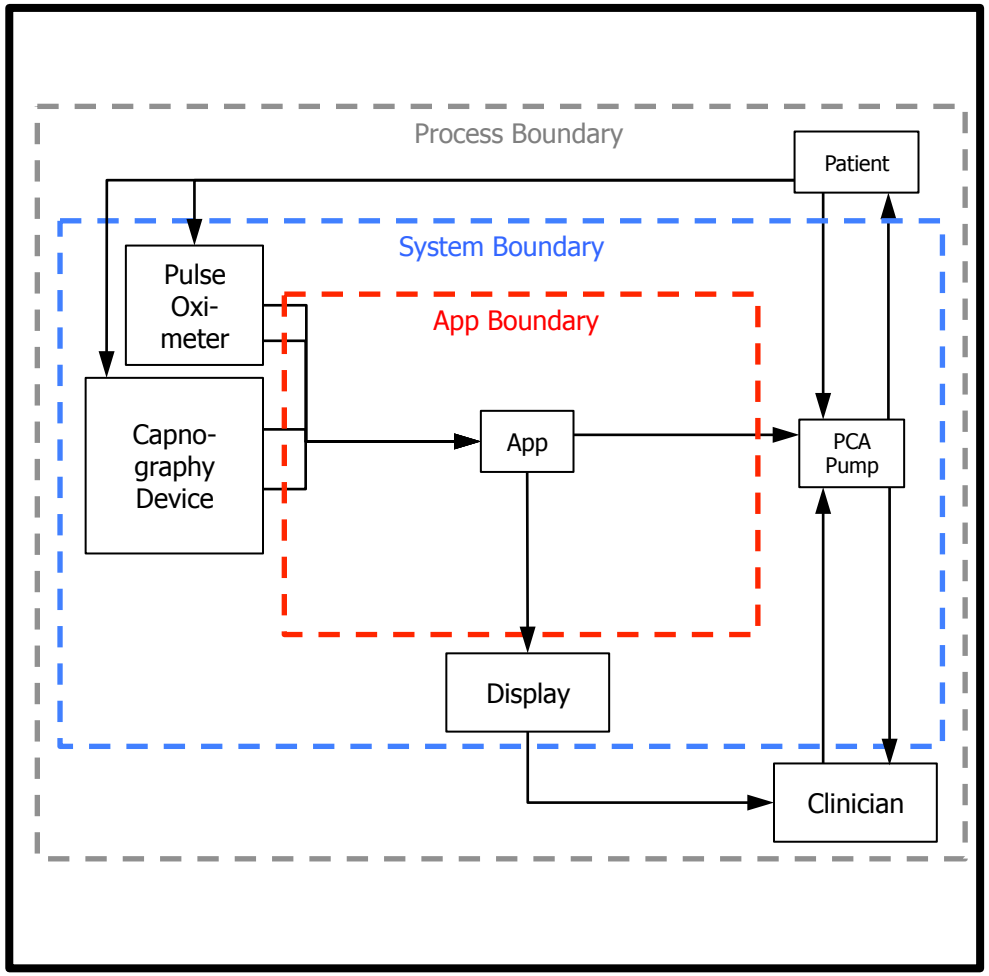

Hazard Analysis

STPA: Fundamentals

- Fundamentals
  - Accident Levels
  - Accidents
  - System Boundaries
  - Hazards
  - Safety Constraints
  - Control Actions
  - Control Structure

Example

1. An inadvertent "Pump Normally" command is sent to the pump [PatientHarmed]

2. Commands are sent to the pump too quickly [PCADoS]

```
InadvertentPumpNormally : constant MAP_Error_Properties::Hazard => [
        Number => 1;
        Description => "An inadvertent `Pump Normally` command is sent to the pump.";
        Accident => PulseOx_Forwarding_Error_Properties::PatientHarmed;
];
```

Hazard Analysis

STPA: Fundamentals

- Fundamentals
  - Accident Levels
  - Accidents
  - System Boundaries
  - Hazards
  - Safety Constraints
  - Control Actions
  - Control Structure

Example

1. The app must only instruct the pump to run at a normal rate when the patient can tolerate more analgesic [InadvertentPumpNormally]

2. The app must wait for a designated length of time between sending pump commands [TooManyCommands]

```
PumpWhenSafe : constant MAP_Error_Properties::Constraint => [
        Number => 1;
        Description => "The app must only instruct the pump to run at a
normal rate when the patient can tolerate more analgesic.";
        Hazard =>
PulseOx_Forwarding_Error_Properties::InadvertentPumpNormally;
    ];
```

Hazard Analysis

STPA: Fundamentals

- Fundamentals
  - Accident Levels
  - Accidents
  - System Boundaries
  - Hazards
  - Safety Constraints
  - Control Actions
  - Control Structure

Example

1. App -> Pump: Pump Normally
2. PulseOx -> App: SpO_2 = 95
3. App -> Display: Patient = Ok

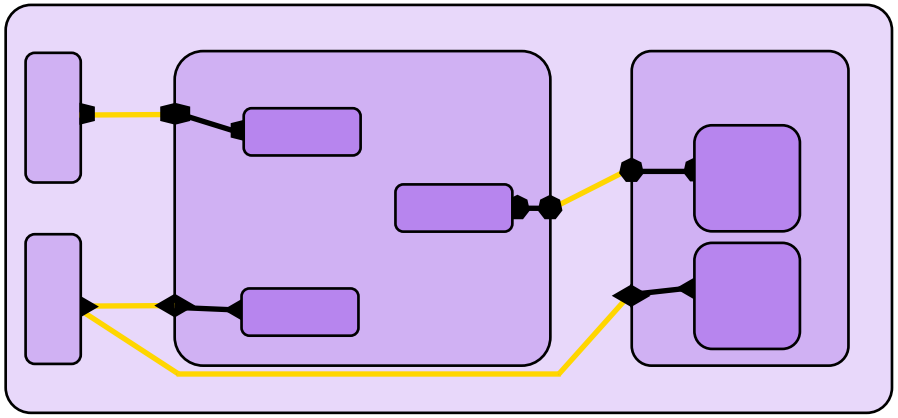

Hazard Analysis

STPA: Fundamentals

- Fundamentals
  - Accident Levels
  - Accidents
  - System Boundaries
  - Hazards
  - Safety Constraints
  - Control Actions
  - Control Structure

Example

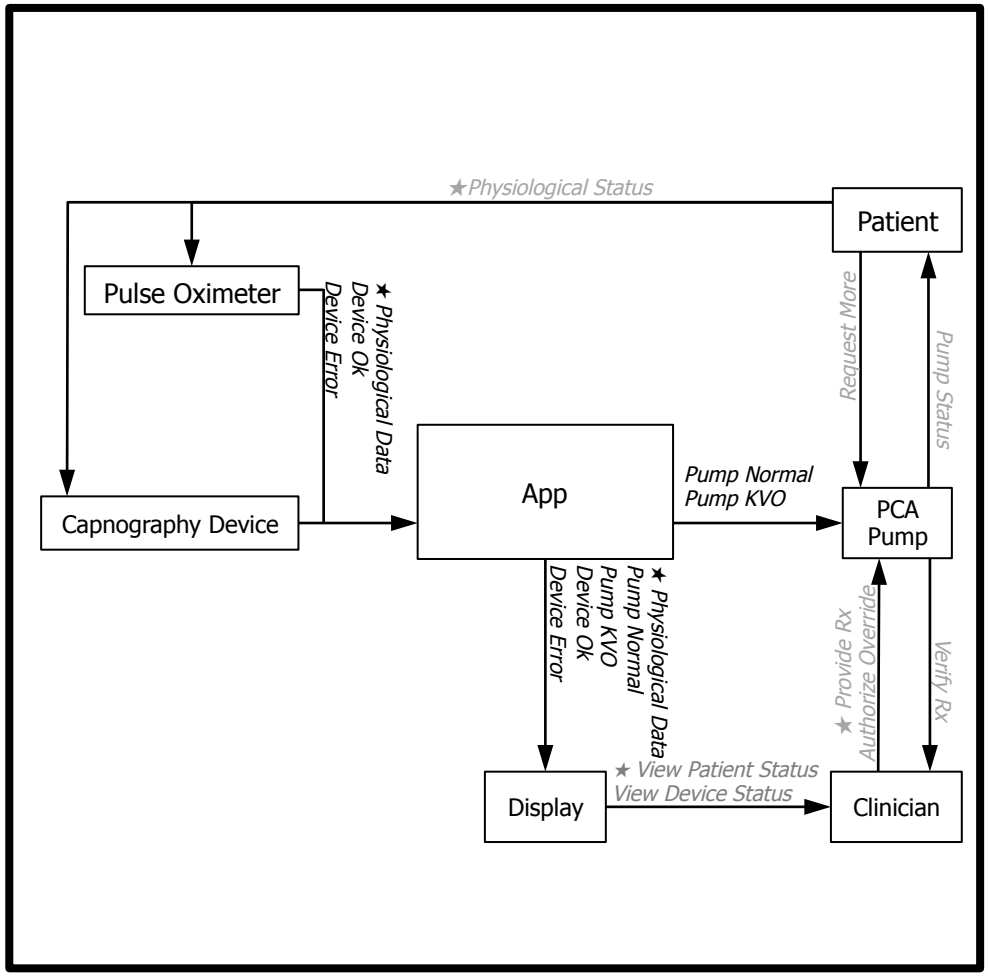

Hazard Analysis

STPA: Identifying Hazardous Control Actions

- Hazardous Control Action Table
  - Cross-product of control actions and STPA guidewords

Control Action	Providing	Not Providing	Applied too Long	Stopped too Soon	Early	Late
App -> Pump: Pump Normally	PH	Not Hazardous	PH	Not Hazardous	PH	Not Hazardous
App -> Disp: Patient Ok	BID	BID	BID	BID	BID	BID
PulseOx->App: Provide SpO_2	Not Hazardous	PH, BID	Not Hazardous	PH, BID	Not Hazardous	PH, BID
PulseOx->App: Provide Pulse Rate	Not Hazardous	PH, BID	Not Hazardous	PH, BID	Not Hazardous	PH, BID

PH = Patient Harmed
BID = Bad Info Displayed

Hazard Analysis

STPA: Hazardous Causes and Compensations

Control Action: App -> Pump: Pump Normally

- Providing:
  - Bad Data:
    - Cause:
      - Incorrect values are gathered from one of the physiological sensors
    - Compensation:
      - Rely on multiple sensed physiological parameters to provide redundancy
- Not Providing:
  - Not hazardous

Hazard Analysis

STPA: Hazardous Causes and Compensations

Control Action: App -> Pump: Pump Normally

- Wrong Timing or Order:
  - Not applicable
- Too Long
  - Network Drop
    - Cause:
      - Network drops out, leaving the pump running normally regardless of the patient's health
    - Compensation:
      - Commands to pump normally have an associated maximum time, after which the pump returns to KVO

STPA Control Loop

Including Causality Guidewords

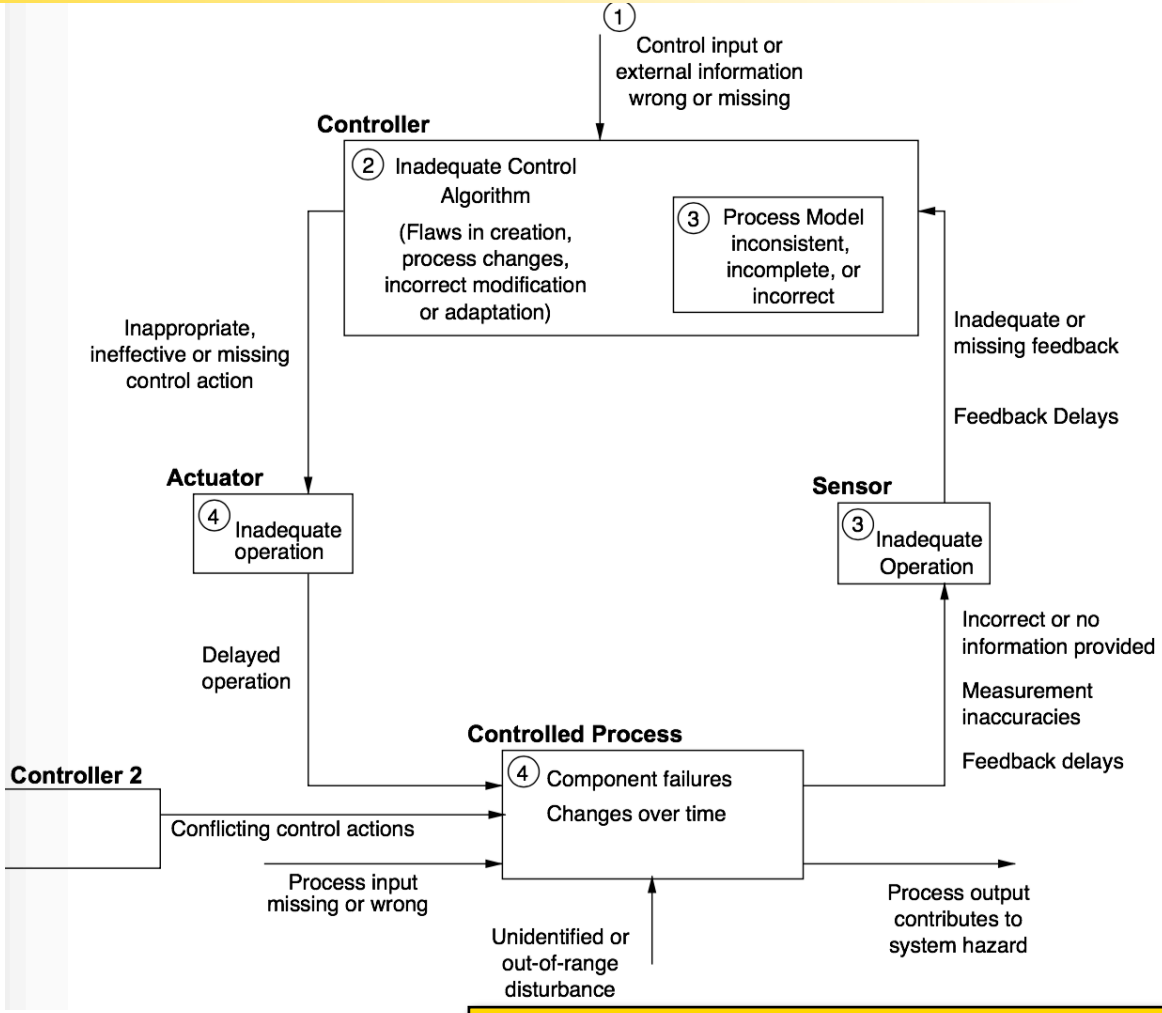

"Engineering a Safer World" Leveson, 2011

Hazard Analysis

Returning to our Architectural Model

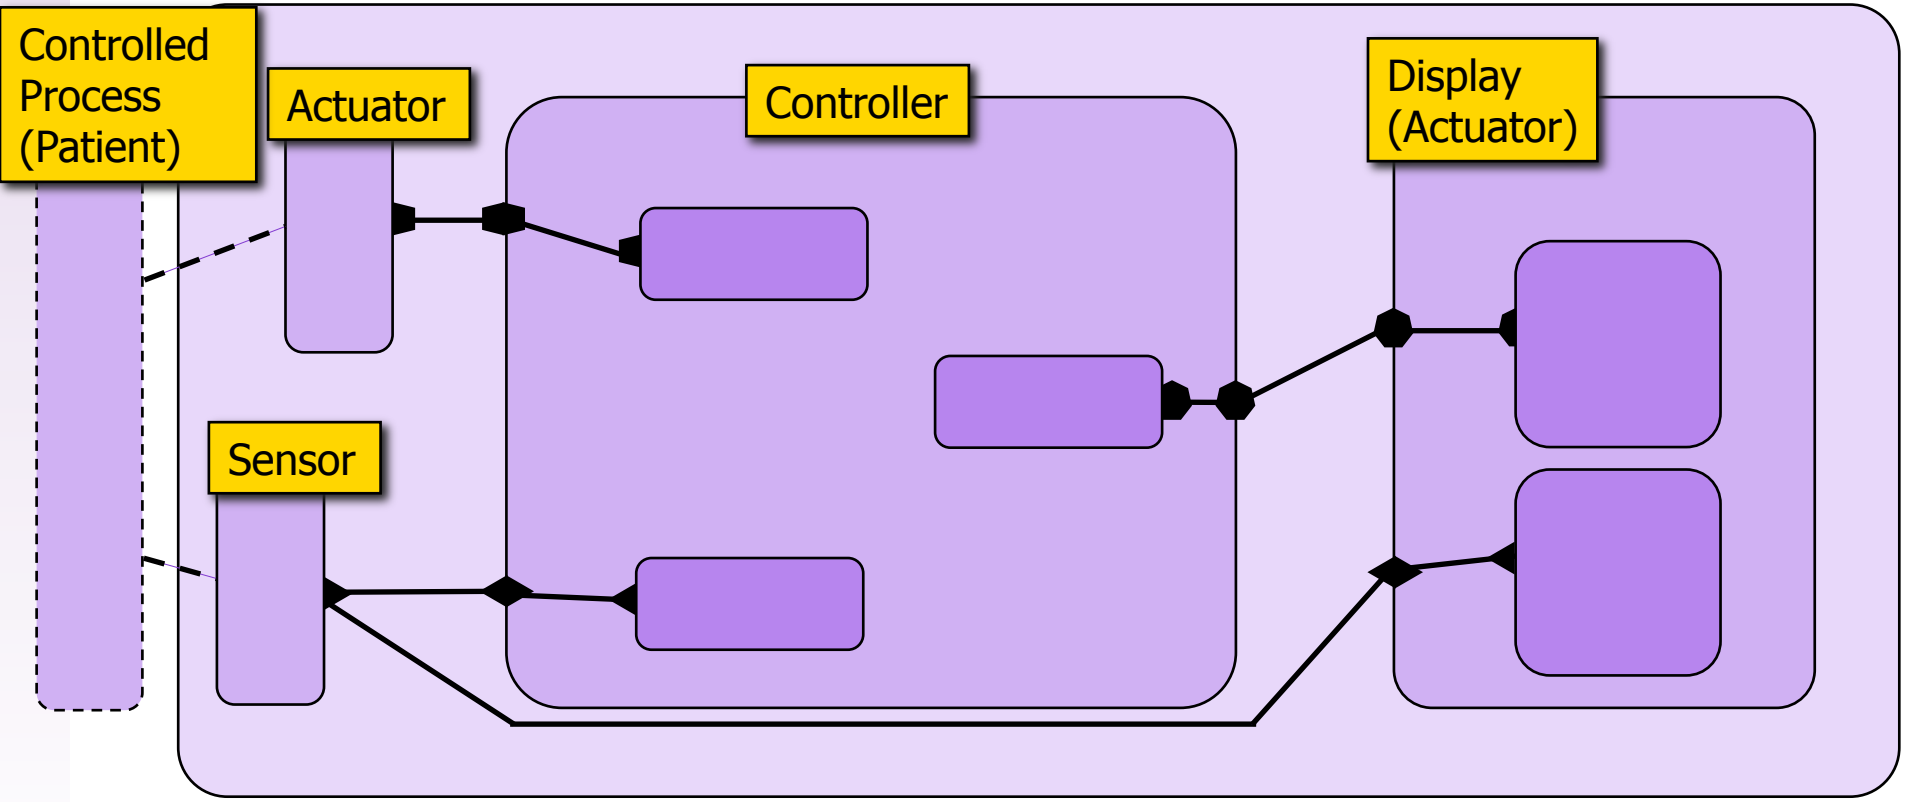

Hazard Analysis

Annotating our Architectural Model

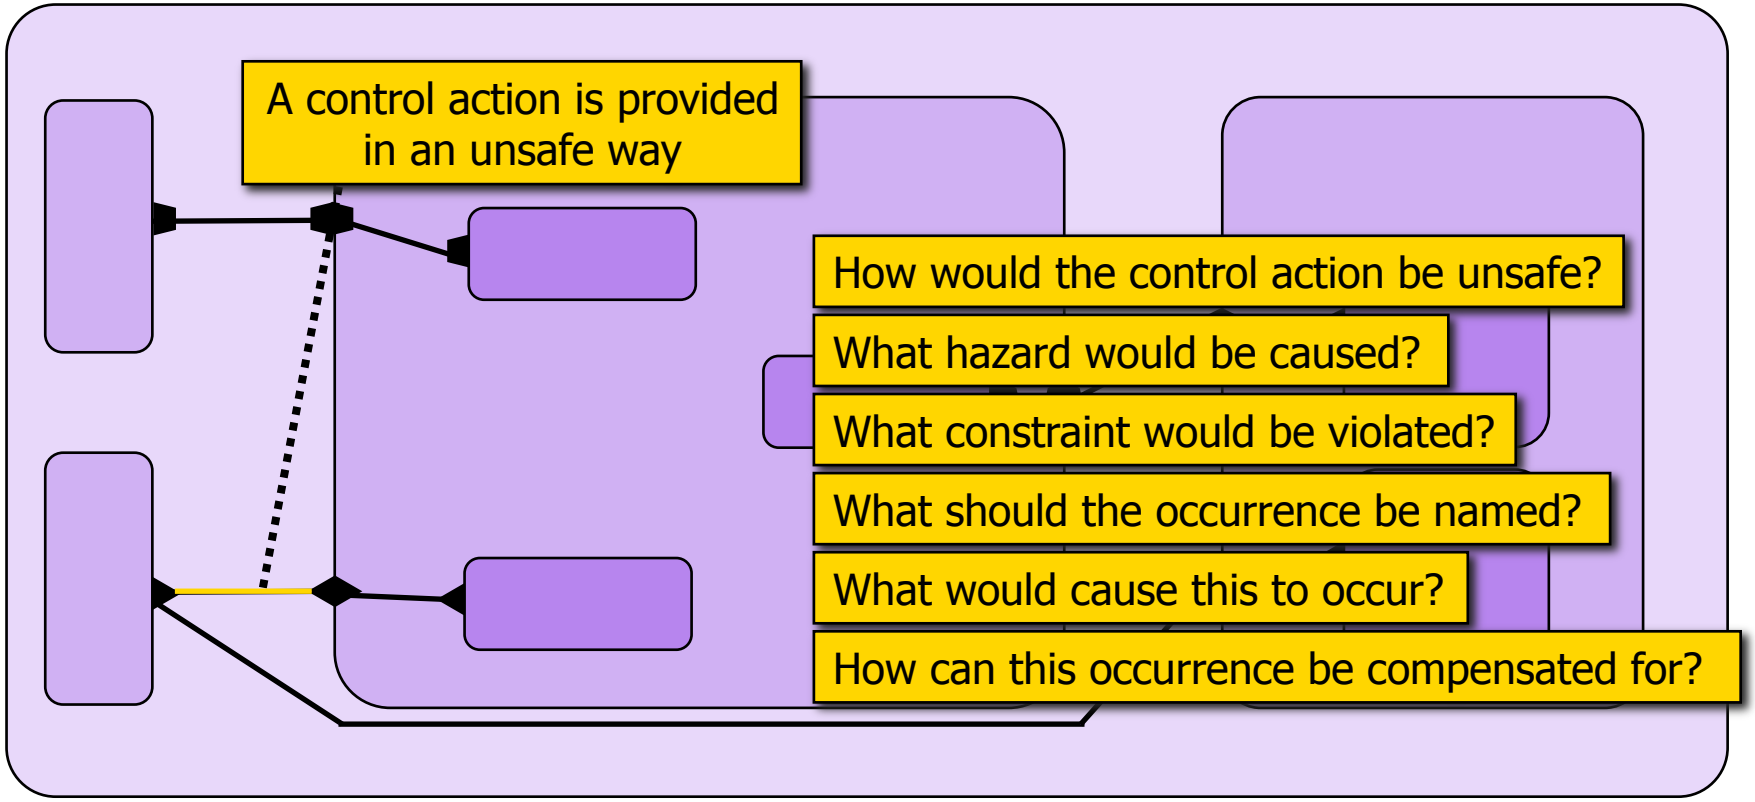

Hazard Analysis

Annotating our Architectural Model

```
package PCA_Shutoff
public

system PCA_Shutoff_System
end PCA_Shutoff_System;

system implementation PCA_Shutoff_System.imp
subcomponents
   pulseOx : device PulseOx_Interface::ICEpoInterfa
   appLogic : process PCA_Shutoff_Logic::ICEpcaShut
connections
   spo2_data : port pulseOx.SpO2 -> appLogic.SpO2;
annex EMV2 {**
   use types PCA_Shutoff_Errors;
   properties
   MAP_Error_Properties::Occurrence => [
      Kind => AppliedTooLong;
      Hazard => PCA_Shutoff_Error_Properties::InadvertentPumpNormally;
      ViolatedConstraint => PCA_Shutoff_Error_Properties::PumpWhenSafe;
      Title => "Network Drop";
      Cause => "Network drops out, leaving the SpO2 value po
      Compensation => "Physiological readings have a maximum                    onger valid";
      Impact => reference(SpO2ValueHigh);
   ] applies to spo2_data;
**};

end PCA_Shutoff_System.imp;
end PCA_Shutoff;
```

How would the control action be unsafe?

What hazard would be caused?

What constraint would be violated?

What should the occurrence be named?

What would cause this to occur?

How can this occurrence be compensated for?

We'll come back to these two in a moment.

Report Generation Development

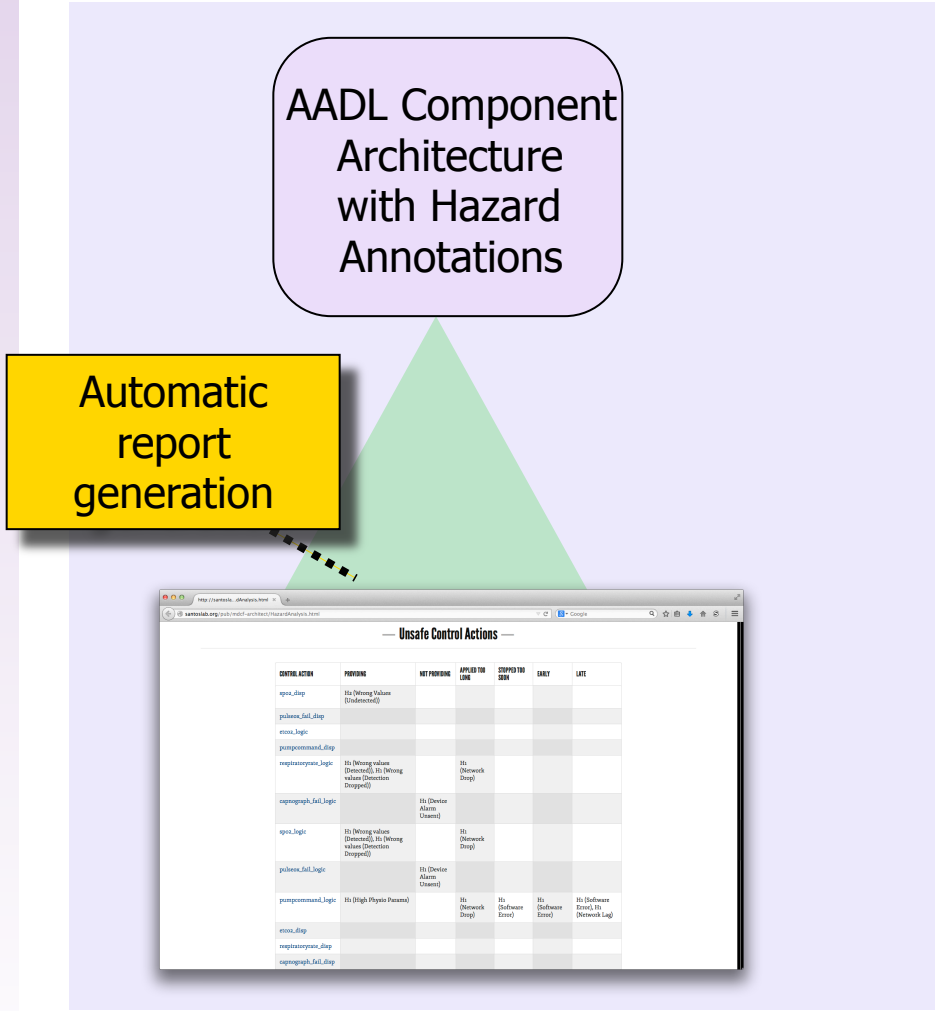

- Development of component architecture using AADL / OSATE2
- Addition of Hazard Analysis Annotations
- Automatic generation of STPA-Styled Hazard Analysis Report

Example "In Progress" Report Online at:
http://santoslab.org/pub/mdcf-architect/HazardAnalysis.html

Annotating our Architectural Model

Inside the AADL System Component

```
package PCA_Shutoff
public

system PCA_Shutoff_System
end PCA_Shutoff_System;

system implementation PCA_Shutoff_System.imp
subcomponents
   pulseOx : device PulseOx_Interface::ICEpoInterface.imp;
   appLogic : process PCA_Shutoff_Logic::ICEpcaShutoffProcess.imp;
connections
   spo2_data : port pulseOx.SpO2 -> appLogic.SpO2;
annex EMV2 {**
   use types PCA_Shutoff_Errors;
   properties
   MAP_Error_Properties::Occurrence => [
      Kind => AppliedTooLong;
      Hazard => PCA_Shutoff_Error_Properties::InadvertentPumpNormally;
      ViolatedConstraint => PCA_Shutoff_Error_Properties::PumpWhenSafe;
      Title => "Network Drop";
      Cause => "Network drops out, leaving the SpO2 value potentially too high";
      Compensation => "Physiological readings have a maximum time, after which they are no longer valid";
      Impact => reference(SpO2ValueHigh);
   ] applies to spo2_data;
**};

end PCA_Shutoff_System.imp;
end PCA_Shutoff;
```

What control action will be affected?

What specific fault will result?

What can we do with our model + specific fault information?

Fault Types

EMV2 Type Hierarchy

Error Library Type	STPA Error Type	App Error Type
Errors with Physiological Monitors		
LateDelivery	DelayedOperation	SpO2ValueLate
IncorrectValue	IncorrectInformation	SpO2ValueLow
N/A	NoInformation	NoSpO2Data
Errors with App Logic		
ServiceCommission	InnapropriateCtrlAction	InadvertentPumpNormally
ServiceOmission	MissingCtrlAction	InadvertentPumpMinimally
AADL Standard Error Types	STPA Error Types	App Specific Error Types

Fault Types

App Specific Error Library

```
package PCA_Shutoff_Errors
public
with MAP_Errors, PCA_Shutoff_Error_Properties, MAP_Error_Properties,
   PCA_Shutoff;

annex EMV2
{**
   error types
   -- These errors aren't associated with unsafe states, but they're here for completeness
   SpO2ValueLow : type extends MAP_Errors::WrongPhysioDataError;
   RespiratoryRateLow : type extends MAP_Errors::WrongPhysioDataError;
   ETCO2ValueHigh : type extends MAP_Errors::WrongPhysioDataError;

   -- These errors will cause the app to logic to think the patient is healthy when she isn't
   SpO2ValueHigh : type extends MAP_Errors::WrongPhysioDataError;
   RespiratoryRateHigh : type extends MAP_Errors::WrongPhysioDataError;
   ETCO2ValueLow : type extends MAP_Errors::WrongPhysioDataError;

   -- These are errors with devices
   DeviceAlarmFailsOn : type extends MAP_Errors::PhysioDeviceErrorCommission;
   DeviceAlarmFailsOff : type extends MAP_Errors::PhysioDeviceErrorOmission;
   BadInfoDisplayedToClinician : type extends MAP_Errors::WrongInfoDisplayedError;
   InadvertentPumpNormally : type extends MAP_Errors::AppCommission;
   InadvertentPumpMinimally : type extends MAP_Errors::AppOmission;
   end types;
**};

end PCA_Shutoff_Errors;
```

Application independent: Sourced from STPA

Application specific: Defined by app risk management process

Hazard Analysis

Annotating the Architectural Model

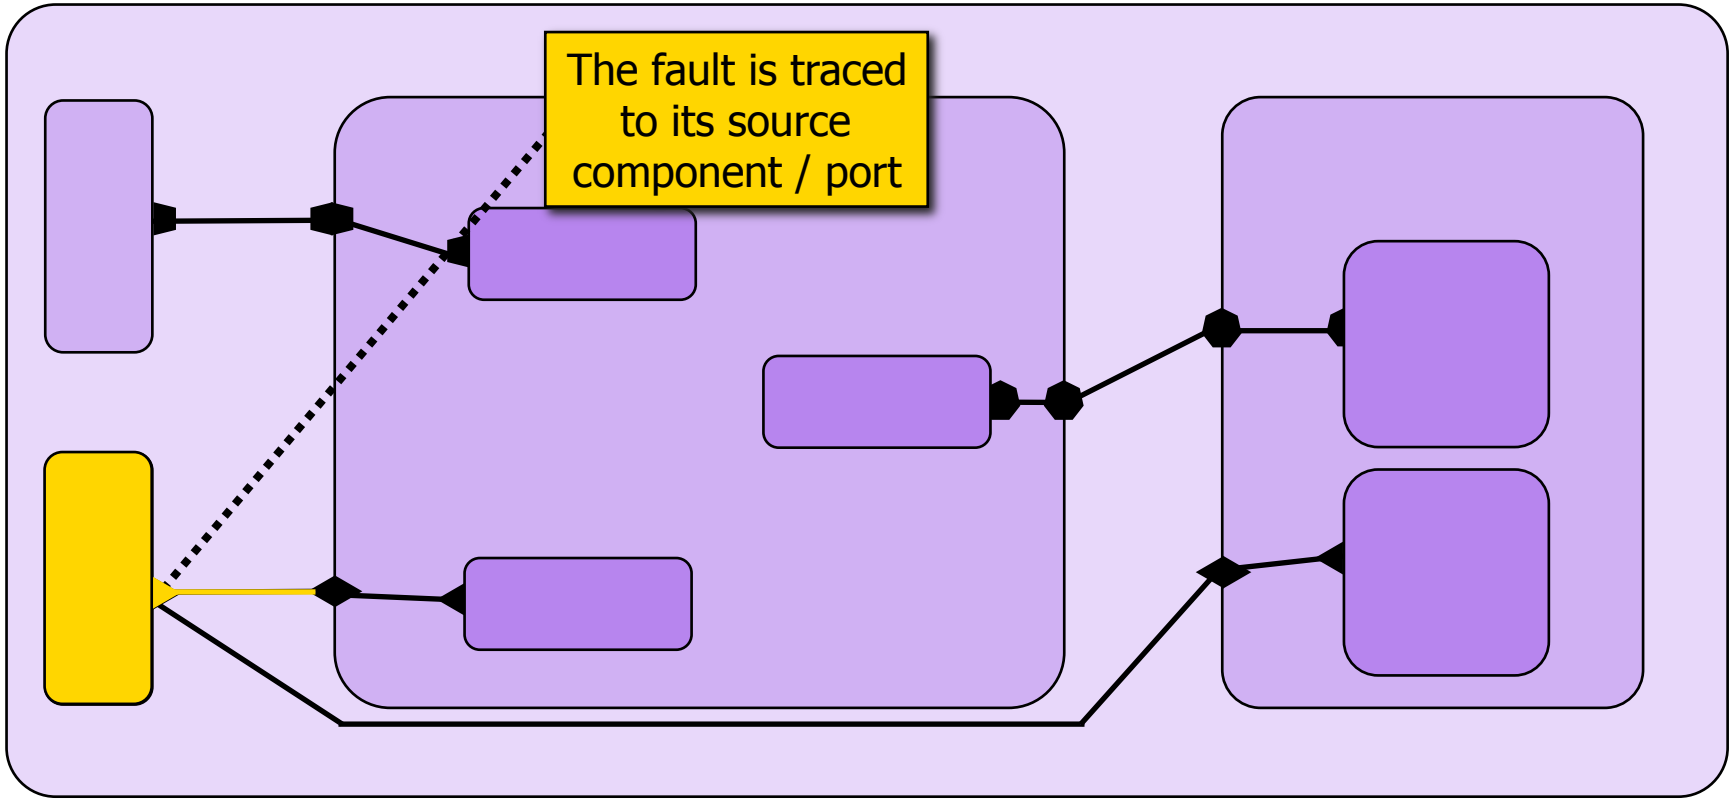

Hazard Analysis

Specification Step 1: Propagation

```
package PulseOx_Interface
public
with PCA_Shutoff_Types, PCA_Shutoff_Errors, EMV2, MAP_Error_Properties, PCA_Shutoff;
   device ICEpoInterface
   features
      SpO2 : out event data port PCA_Shutoff_Types::SpO2;
   annex EMV2 {**
      use types PCA_Shutoff_Errors;
      error propagations
         SpO2 : out propagation {SpO2ValueHigh};
         flows
            SpO2UnDetectableHighValueFlowSource : error source SpO2 {SpO2ValueHigh};
      end propagations;
   **};
   end ICEpoInterface;

   device implementation ICEpoInterface.imp
   end ICEpoInterface.imp;

end PulseOx_Interface;
```

Port the fault will propagate on

Specific Fault

Direction of the propagation

Hazard Analysis

Specification Step 2: Flow

```
package PulseOx_Interface
public
with PCA_Shutoff_Types, PCA_Shutoff_Errors, EMV2, MAP_Er[illegible]PCA_Shutoff;
   device ICEpoInterface
   features
      SpO2 : out event data port PCA_Shutoff_Types::SpO2;
   annex EMV2 {**
      use types PCA_Shutoff_Errors;
      error propagations
         SpO2 : out propagation {SpO2ValueHigh};
         flows
            SpO2UnDetectableHighValueFlowSource : error source SpO2 {SpO2ValueHigh};
      end propagations;
   **};
   end ICEpoInterface;

   device implementation ICEpoInterface.imp
   end ICEpoInterface.imp;

end PulseOx_Interface;
```

Name of flow

Specific port

Specific fault

Type of flow

Hazard Analysis

Error transformation

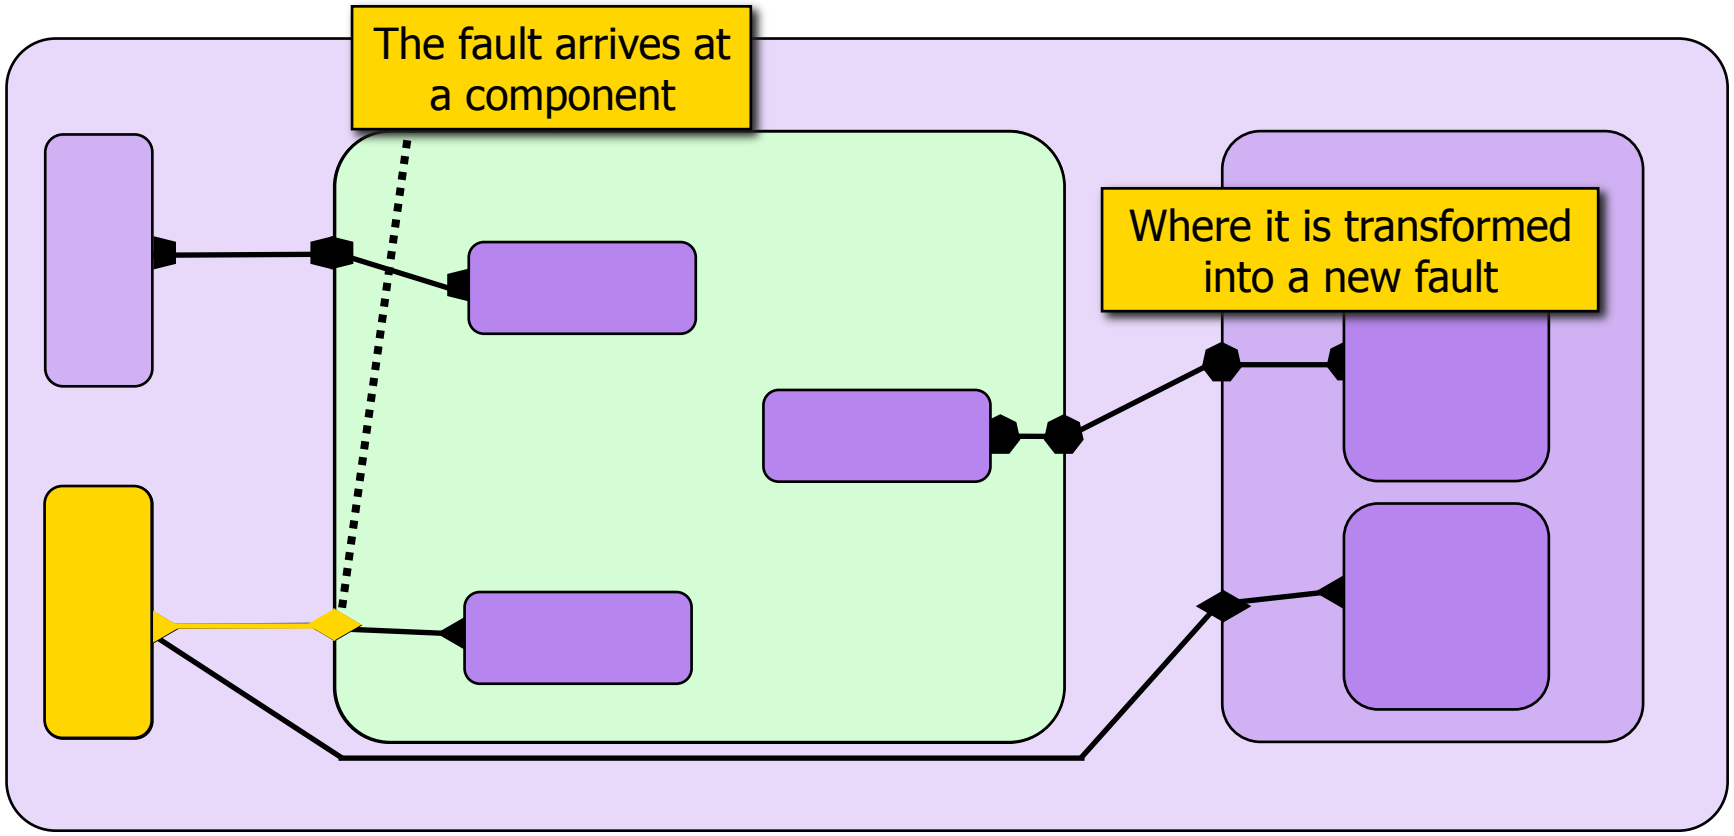

Hazard Analysis

Specification Step 3: Error Transformations

```
package PCA_Shutoff_
public
with PCA_Shutoff_Types, PCA_Shutoff_Properties, MAP_Properties;

   process ICEpcaShutoffProcess
   features
      SpO2 : in event data port PCA_Sh
      CommandPumpNormal : out event data port PCA_Shutoff_Types::PumpNormalCommand;
   properties
      MAP_Properties::Component_Type => logic;
   annex EMV2 {**
      use types PCA_Shutoff_Errors;
      error propagations
         SpO2 : in propagation {SpO2ValueHigh};
         CommandPumpNormal : out propagation {InadvertentPumpNormally};
         flows
            HighSpO2LeadsToOD : error path SpO2{SpO2ValueHigh} -> CommandPumpNormal{InadvertentPumpNormally};
      end propagations;
   **};
   end ICEpcaShutoffProcess;

   -- Process implementation redacted
end PCA_Shutoff_Logic;
```

Incoming Port

Incoming Fault

Outgoing Port

Outgoing Fault

Hazard Analysis

Specification Step 3: Error Transformations

```
package PCA_Shutoff_Logic
public
with PCA_Shutoff_Types, PCA_Shutoff_Properties, MAP_Properties;

   process ICEpcaShutoffProcess
   features
      SpO2 : in event data port PCA_Shutoff_Types::SpO2;
      CommandPumpNormal : out event data port PCA_Shutoff_Types::PumpNormal
   properties
      MAP_Properties::Component_Type =>
   annex EMV2 {**
      use types PCA_Shutoff_Errors;
      error propagations
         SpO2 : in propagation {SpO2ValueHigh};
         CommandPumpNormal : out propagation {InadvertentPumpNormally};
         flows
            HighSpO2LeadsToOD : error path SpO2{SpO2ValueHigh} -> CommandPumpNormal{InadvertentPumpNormally};
      end propagations;
   **};
   end ICEpcaShutoffProcess;

   -- Process implementation redacted
end PCA_Shutoff_Logic;
```

Name of flow

Type of flow

Specific faults

Specific Ports

Hazard Analysis

Error Sinks

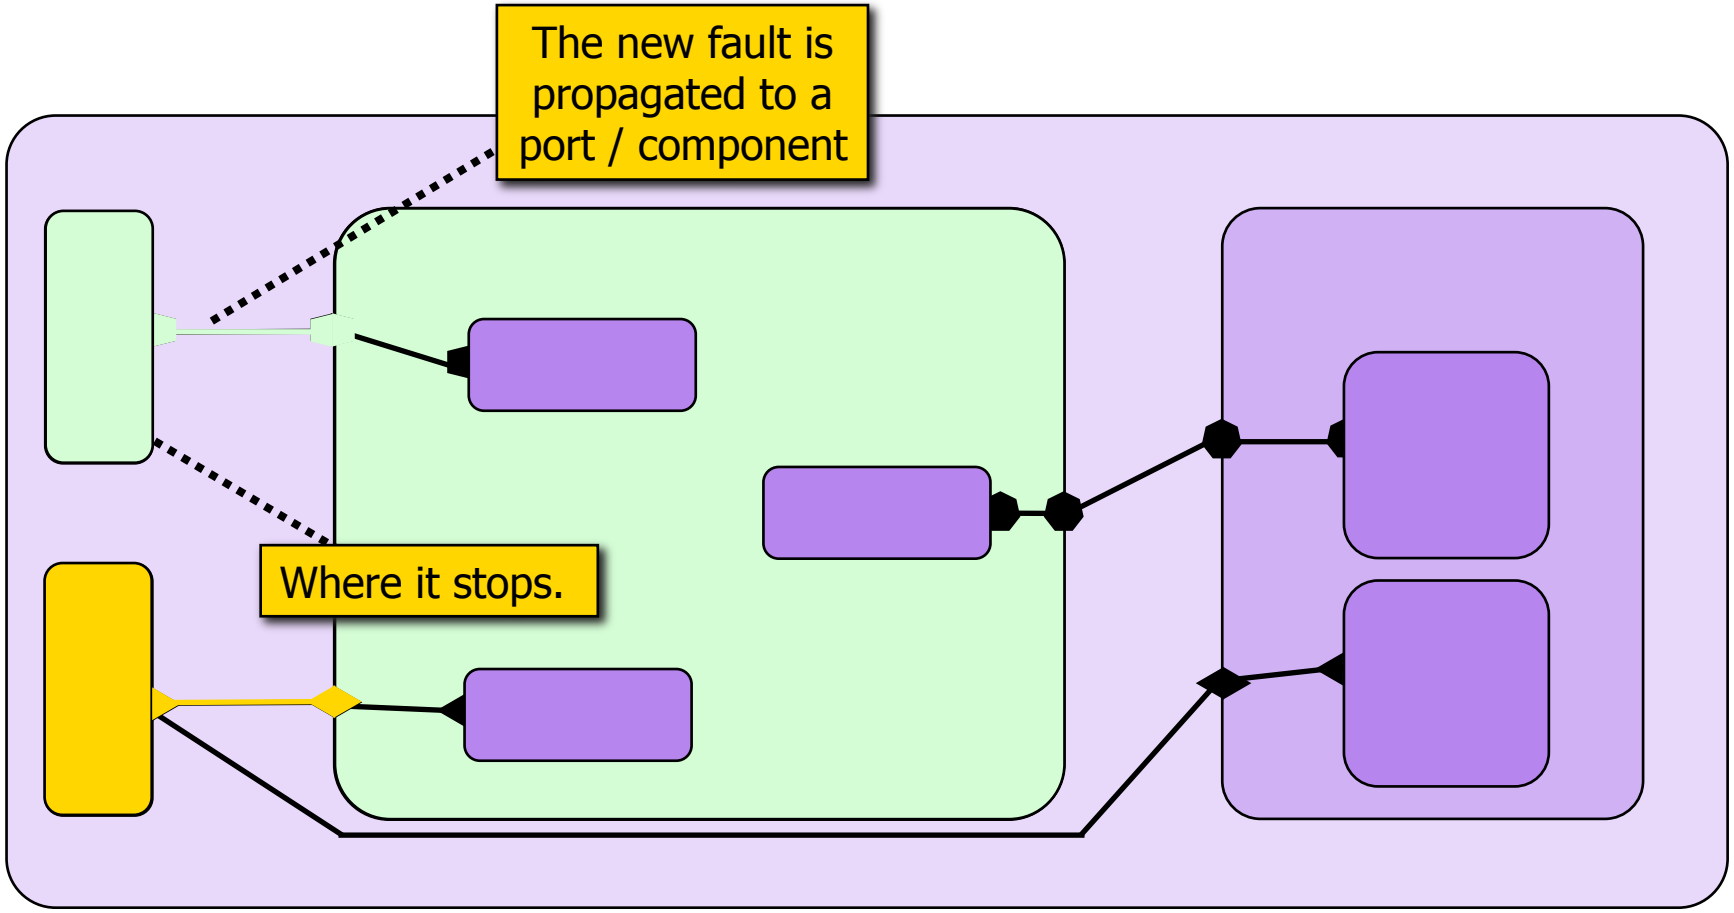

Hazard Analysis

Specification Step 4: Error Sink

Port the fault will arrive on

Specific fault type

```
package PCAPump_Interface
public
with PCA_Shutoff_Types;
   device ICEpcaInterface
   features
      PumpNormally : in event data port PCA_Shutoff_Types::PumpNormalCommand;
   annex EMV2 {**
      use types PCA_Shutoff_Errors;
      error propagations
         PumpNormally : in propagation {InadvertentPumpNormally};
         flows
            ODCommand : error sink PumpNormally {InadvertentPumpNormally};
      end propagations;
   **};
   end ICEpcaInterface;

   device implementation ICEpcaInterface.imp
   end ICEpcaInterface.imp;

end PCAPump_Interface;
```

Hazard Analysis

Specification Step 4: Error Sink

```
package PCAPump_Interface
public
with PCA_Shutoff_Types;
   device ICEpcaInterface
   features
      PumpNormally : in event data port PCA_Shutoff_Types::Pu
   annex EMV2 {**
      use types PCA_Shutoff_Errors;
      error propagations
         PumpNormally : in propagation {InadvertentPumpNormally};
         flows
            ODCommand : error sink PumpNormally {InadvertentPumpNormally};
      end propagations;
   **};
   end ICEpcaInterface;

   device implementation ICEpcaInterface.imp
   end ICEpcaInterface.imp;

end PCAPump_Interface;
```

Name of flow

Type of flow

Specific fault

Specific Port

Hazard Analysis

OSATE Remembers a Neglected Connection

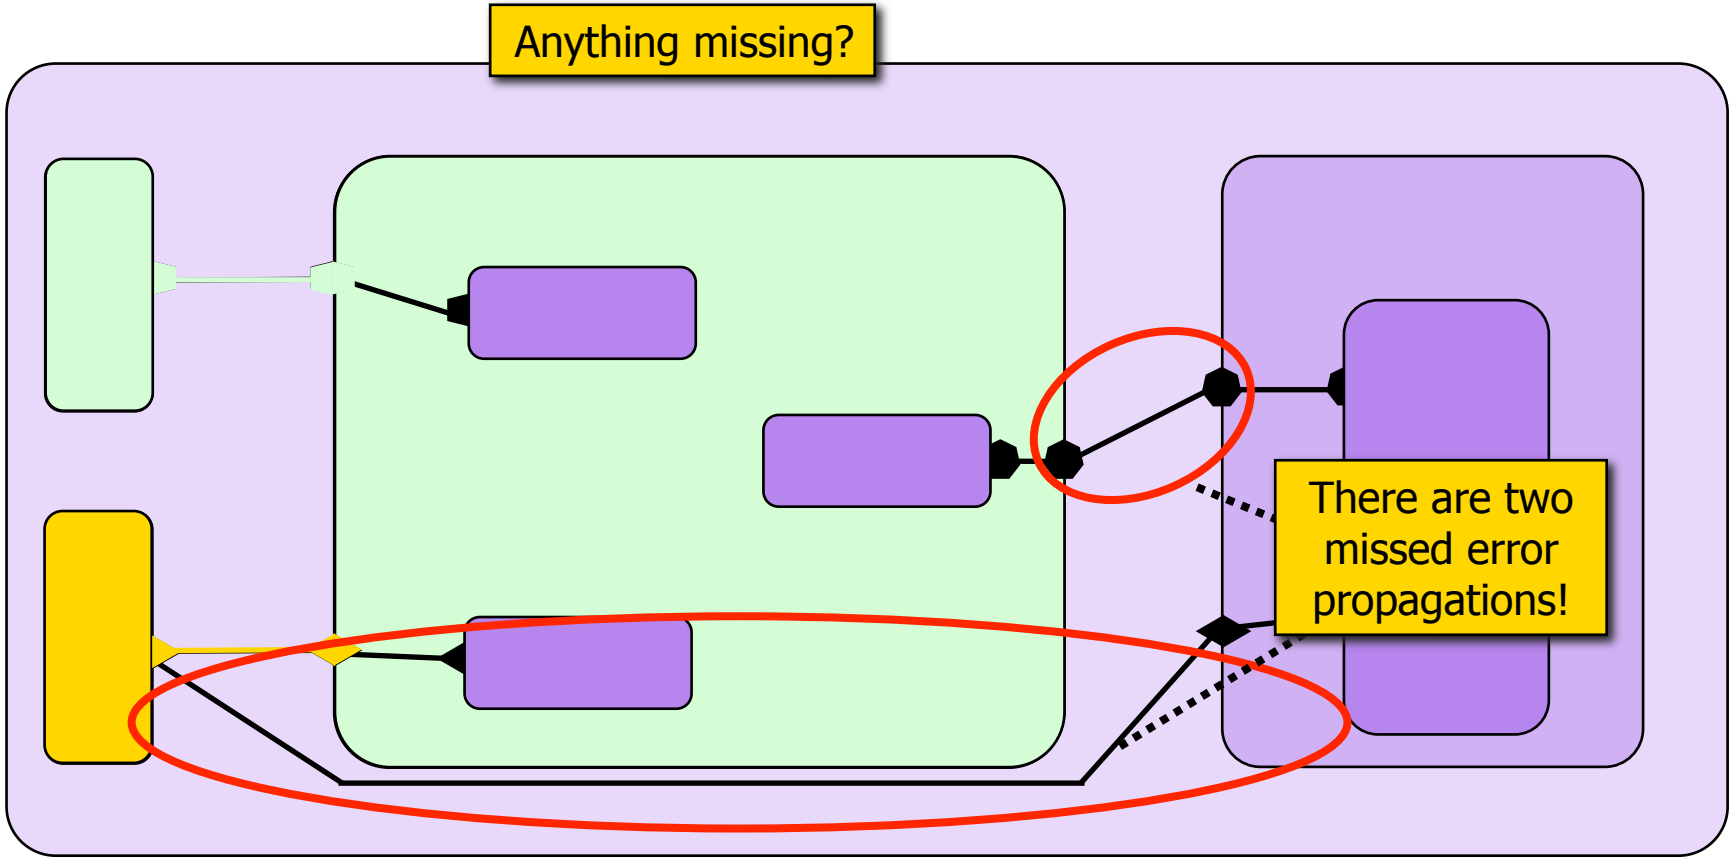

Hazard Analysis

OSATE Remembers A Neglected Connection

```
system implementation PCA_Shutoff_System.imp
subcomponents
    -- Physiological inputs
    pulseOx : device PulseOx_Interface::ICEpoInterface.imp;

    -- App logic
    appLogic : process PCA_Shutoff_Logic::ICEpcaShutoffProcess.imp;
    appDisplay : process PCA_Shutoff_Display::ICEpcaDisplayProcess.imp;
connections
    -- From components to logic
    spo2_logic : port pulseOx.SpO2 -> appLogic.SpO2;

    -- From components to display
    spo2_disp : port pulseOx.SpO2 -> appDisplay.SpO2;
anne
```

No incoming error propagation from appDisplay for outgoing propagation SpO2{SpO2ValueHigh}. Check for Unhandled Faults.

```
    properties
    -- Errors between the PulseOx's SpO2 channel and the App Logic
    MAP_Error_Properties::Occurrence => [
        Kind => ValueHigh;
        Hazard => PCA_Shutoff_Error_Properties::PatientHarmed;
        ViolatedConstraint => PCA_Shutoff_Error_Properties::PumpWhenSafe;
        Title => "Wrong Values (Undetected)";
        Cause => "Incorrect values are gathered from the physiological sensors";
```

Tool

OSATE2

- Open-source, Eclipse-based tool
- Our work is available as a plugin
  - Uses the model-traversal built into OSATE2

Open Source AADL
Tool Environment

http://www.aadl.info
http:/www.aadl.info/wiki

Hazard Analysis

Our model is updated accordingly

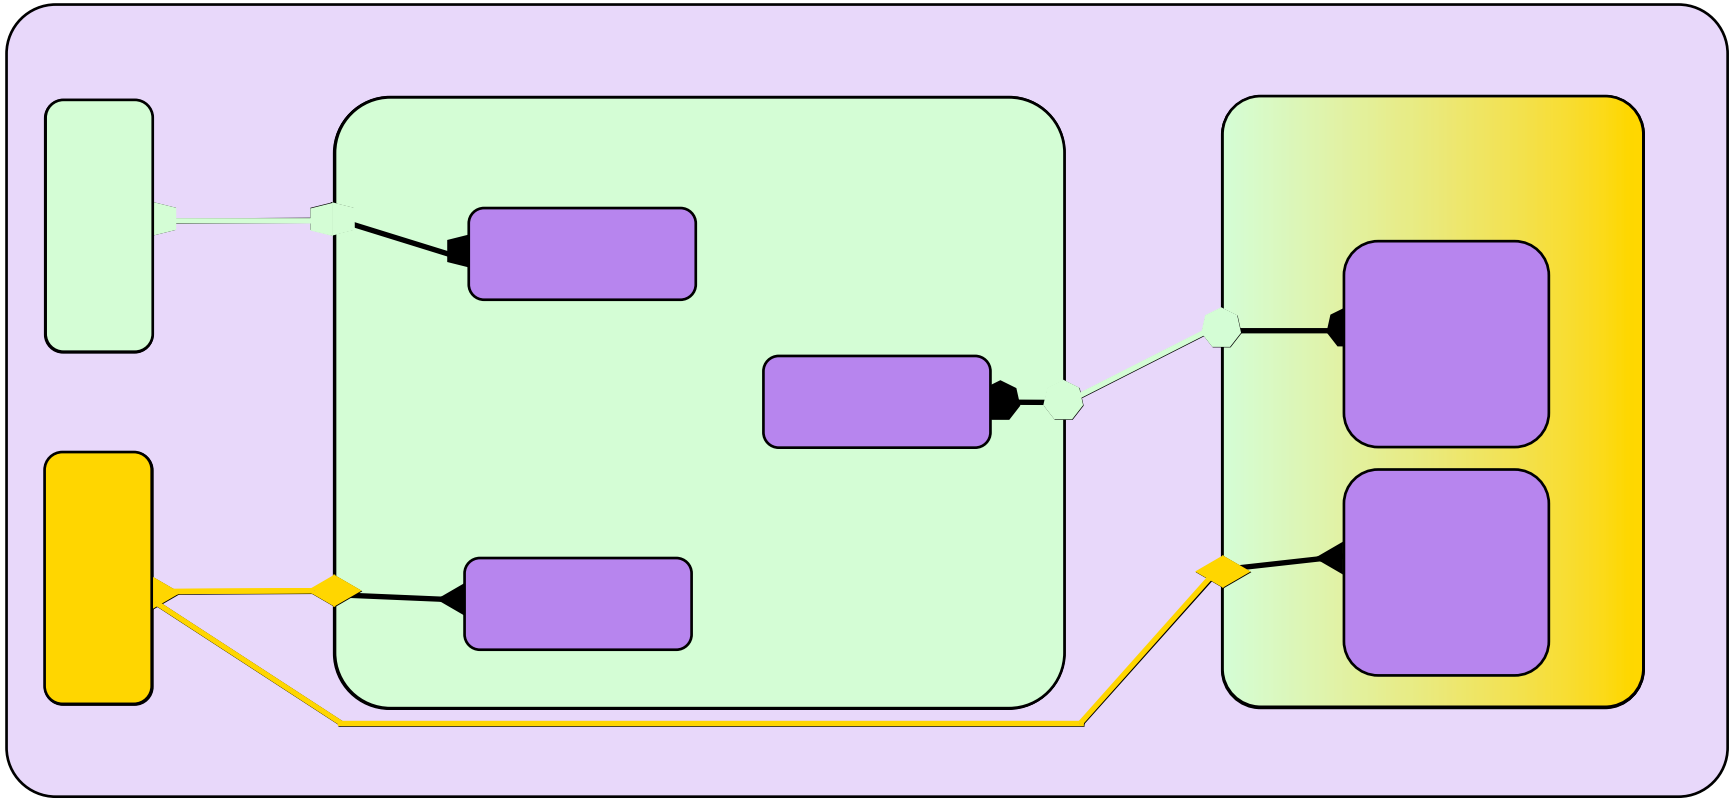

Hazard Analysis

Interaction between Report and Model

CONTROL ACTION	PROVIDING	NOT PROVIDING	APPLIED TOO LONG	STOPPED TOO SOON	EARLY	LATE
spo2_disp	H2 (Wrong Values (Undetected))					
pulseox_fail_disp						
etco2_logic						
pumpcommand_disp						
respiratoryrate_logic	H1 (Wrong values (Detected)), H1 (Wrong values (Detection Dropped))		H1 (Network Drop)			
capnograph_fail_logic		H2 (Alarm Unsent)				
spo2_logic	H1 (Wrong values (Detected)), H1 (Wrong values (Detection Dropped))		H1 (Network Drop)			

Bottom Up

Top Down

1. Here's an empty cell (STPA Keyword + Control Action)… could anything go wrong?

2. Create occurrence and supporting EMV2 annotations

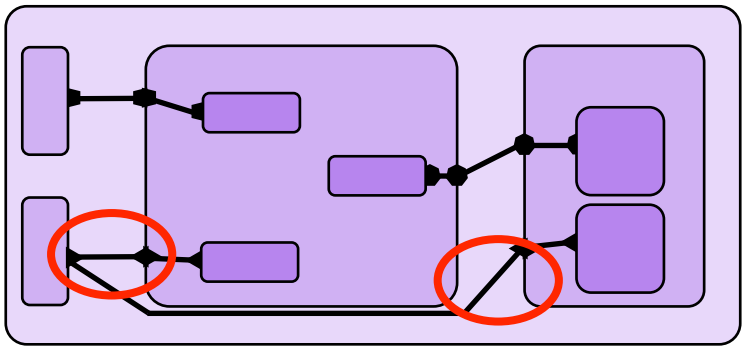

3. Where else could this fault go?

4. What else could cause this error?

Outline

- Background
- Status Quo
- STPA + AADL
- Impacts / Future

Contributions (1 of 2)

- Showing how STPA methods / artifacts can be integrated with a formal architecture modeling framework
- Demonstrating how AADL EM annotations can aid in supporting STPA
- Demonstrating a methodology for carrying out STPA in AADL-defined architectures

Contributions (2 of 2)

- Tool support to automate parts of the methodology
  - And to aid both analysts and reviewers in analysis and review of the generated STPA artifacts.
- Establishing the basis for very strong traceability between
  - Requirements,
  - Architecture,
  - Hazard analysis,
  - Testing / Verification, and
  - Executable code

Further Reading

- Source available online at https://github.com/santoslab/aadl-translator
- Installable into OSATE2 via update site: http://santoslab.org/pub/mdcf-architect/updatesite
- Full documentation online at http://santoslab.org/pub/mdcf-architect
- Publications online at http://people.cis.ksu.edu/~samprocter

Towards Assurance of a Patient-Specific Network of Medical Devices.

SCC 2015, Rockville Maryland

Sam Procter, John Hatcliff, and Robby
SAnToS Lab
Kansas State University

Support:

This work is supported in part by the US National Science Foundation (NSF) (#1239543), the NSF US Food and Drug Administration Scholar-in-Residence Program (#1355778) and the National Institutes of Health / NIBIB Quantum Program.